

GETTING STARTED WITH MINIMED™ 670G **INSULIN PUMP**



Medtronic





The MiniMed 670G Insulin Pump

■ Getting started with the MiniMed 670G Insulin Pump

- Section 1: Welcome..... 1
- Section 2: Pump mechanics and the delivery of insulin 2
- Section 3: Pump basics 4
 - The front of your pump 4
 - The bottom of your pump 5
 - The back of your pump..... 5
 - Attaching the skins..... 5
 - Inserting the battery 5
- Section 4: Startup Wizard 7
- Section 5: Home screen 8
 - Status icons 8
 - Unlocking the pump 9
 - Backlight..... 9
- Section 6: Menu..... 10
 - Menu options 10
- Section 7: Main menu items—a closer look 14
 - Audio Options..... 14
 - Display Options 15
- Section 8: Basal Patterns 16
 - Basal Pattern Setup—one basal rate 16
 - Basal Pattern Setup—changing a basal rate..... 19
 - Basal Pattern Setup—multiple basal rates 20
 - Basal Pattern Setup—removing basal rates 24
 - Suspend Delivery 25
- Section 9: Giving boluses 28
 - Giving a manual bolus 28
 - Stopping a bolus that you have started..... 29
 - Bolus Wizard..... 31



Contents

| | |
|--|-----------|
| Using the Bolus Wizard..... | 35 |
| Status..... | 38 |
| Checking last bolus | 39 |
| Checking bolus history | 40 |
| Section 10: Using the compatible Ascensia BG meter | 41 |
| Charging your meter | 41 |
| Introduction to CareLink Personal software | 42 |
| Section 11: Frequently asked questions..... | 43 |
| Where should I wear my pump? | 43 |
| Where can I put the pump when I sleep? | 43 |
| What about intimacy?..... | 43 |
| Should the pump be removed for X-rays, CT scans, and MRIs? | 44 |
| What do I need to know about traveling with my insulin pump? | 44 |
| When should I call my healthcare professional? | 47 |
| Section 12: Additional features for experienced users | 49 |
| Dual Wave and Square Wave bolus..... | 49 |
| Square Wave..... | 49 |
| Dual Wave | 51 |
| Temp Basal | 54 |
| Adding new or copying Basal Patterns | 57 |
| Basal Patterns Review..... | 58 |
| Max Basal/Max Bolus..... | 60 |
| Auto Suspend | 62 |
| ■ Training handouts | |
| Safety Rules Quick Reference Guide | 65 |
| Alerts | 67 |
| Alarms | 68 |
| Basal Quick Reference Guide | 69 |
| Bolus Wizard™ Quick Reference Guide | 72 |
| Changing the Quick-set™ infusion set | 75 |
| Connecting the pump and meter | 80 |



Welcome

Getting started with the MiniMed 670G Insulin Pump

Section 1: Welcome

Welcome! We are glad that you have chosen insulin pump therapy and are excited for you to begin using your insulin pump.

Whether you've chosen pump therapy because of its convenience, the flexibility it provides, or to help improve your glucose control, your pump will be a valuable tool in helping to manage your diabetes.

This guide provides step-by-step instructions on the basic operation and programming of your pump. Using your pump to complete each practice exercise will help you become comfortable with the basics and prepare you for your in-person training. The information is presented in an order that will build your skills and knowledge.



Note: Did you know that a complete explanation of the technical and operational aspects of your pump can be found in the *MiniMed 670G System User Guide*?

During your in-person training, your trainer will build on this information and help ensure that you are confident to begin pump therapy.

Here are some quick tips to keep in mind as you work through this information:

- Be sure you are not attached to your new insulin pump while you practice.
- If you press the wrong button, press the  button to go back to the previous screen and try again.
- If you do not touch a button for 15 seconds, the pump screen will turn dark. Press any button and the pump screen will return.
- Avoid the Reservoir & Tubing screen until you have completed all practice necessary to feel comfortable using this insulin pump.

We hope you enjoy learning about your new insulin pump.




WARNING: Do not insert the reservoir until you have been instructed to do so by your healthcare professional and have received formal training with a certified product trainer. Attempting to use insulin in your pump before you have received training may result in the delivery of too little or too much insulin, which can cause hyperglycaemia or hypoglycaemia.



Section 2: Pump mechanics and the delivery of insulin

Before we begin, let's make sure you know how insulin is delivered when using an insulin pump. The parts that make up the pump's delivery system are the infusion set, the reservoir, and the pump.

- 1 Tubing
- 2 Reservoir connector
- 3 Insertion site section
- 4 Cannula
- 5 Adhesive
- 6 Reservoir compartment

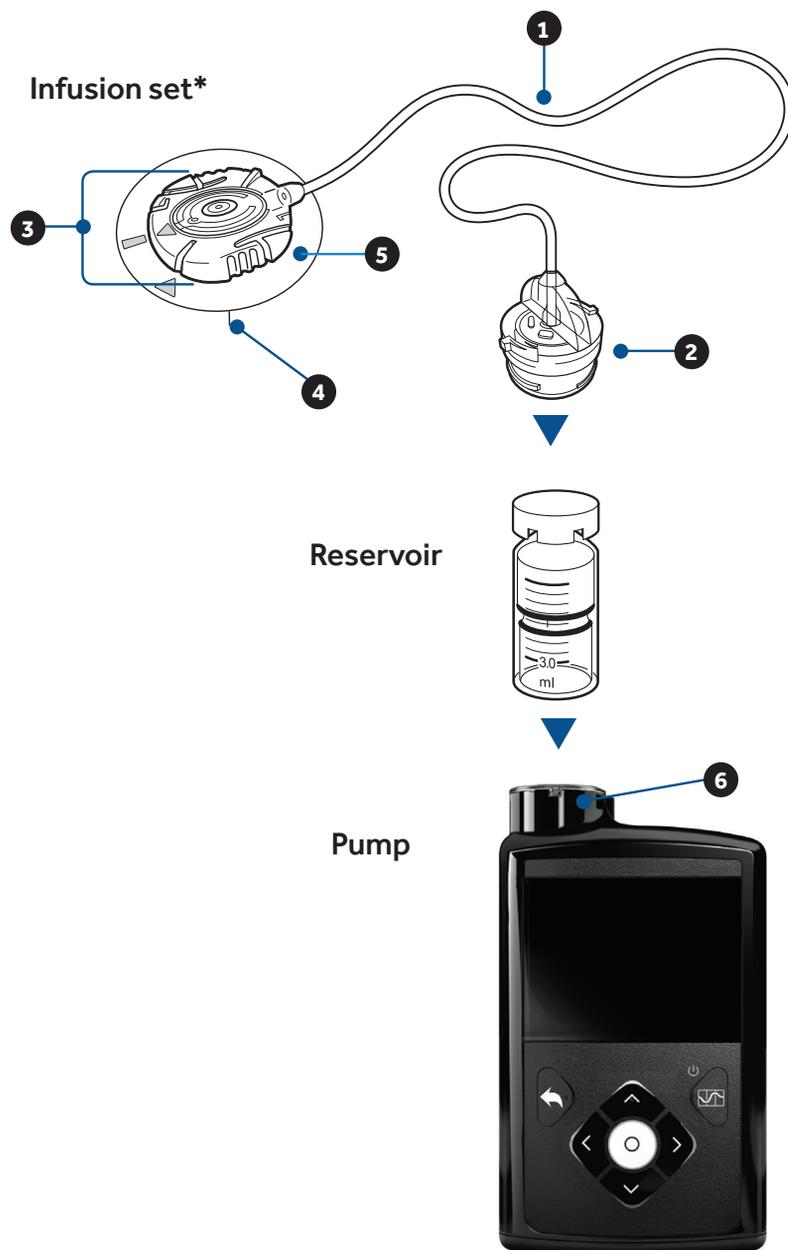

*Quick-set infusion set shown in illustration.



Getting started | Pump mechanics and the delivery of insulin

Infusion set

The infusion set consists of tubing (1) that carries insulin from the pump to you. On one end of the tubing is the reservoir connector (2) that attaches to the reservoir which holds the insulin. On the other end is the insertion site section (3) that attaches to you.

The insertion site section has a small insertion needle that places a tiny flexible tube called a cannula (4) into your body*. Once the infusion set is inserted, you remove the needle, leaving just the cannula behind. A small piece of adhesive (5) holds the infusion set in place. Replace the infusion set every 2 to 3 days. Insulin is not labeled for more than three days when it is used in an infusion set.

Reservoir

The reservoir fits into the pump's reservoir compartment (6). Replace your reservoir and infusion set at the same time.

Pump

Inside the pump, at the bottom of the reservoir compartment, is a piston. The piston acts like the plunger rod on a syringe, pushing up on the bottom of the reservoir, moving insulin into the tubing, through the cannula, and into your body.

The piston is controlled by a mini computer inside the pump that's able to deliver insulin in very small doses, as small as 0.025 units. **It must be rewound each time a newly filled reservoir is placed into the reservoir compartment.**

*Some infusion sets do not use a cannula but have a small needle that remains inserted in the body.

Section 3: Pump basics

Before inserting the battery or pressing any buttons, let's take a closer look at your pump.

The front of your pump

Up, Down, Left, and Right

- Press to scroll up or down through a menu or list.
- Press to move to the desired area on the screen.
- Press to change the value in an area.
- Press to unlock your pump when it has been in Sleep mode.

Back

- Press to return to a previous screen.
- Press and hold to return to the starting screen, called the Home screen.

Select

- Press to select or confirm a value or menu option that is highlighted.
- Press when directions say select.
- Press to access the menu when you are on the Home screen.

Graph

- Press and hold to put the pump into Sleep mode.

Notification light

- Flashes when an alert or an alarm is occurring.



The bottom of your pump



Medtronic Diabetes 24 Hour HelpLine telephone number

For product assistance, call this number to be routed to your local support team.

The back of your pump



Pump serial and model number

You may need to provide these numbers if you call for assistance.

Attaching the skins

Skins are designed to attach to the back of the pump and the front of the pump clip. In addition to personalising the look of your pump, skins provide additional protection against surface scratches. Apply the skins using the instructions provided with them.



Note: Not all countries include the skins kit with your system order. To order a skins kit, contact your local representative.

Inserting the battery

Your insulin pump is powered by a AA battery. A lithium, alkaline, or rechargeable AA battery can be used. The battery you place into your pump should always be new or fully charged.




Note: Lithium batteries have been shown to have the longest battery life. Batteries should be stored at room temperature, not in the refrigerator or other cold locations.

To insert the battery and get started, you will need the:

- Battery cap found with the pump
- Pump clip found with the accessories
- AA battery found with the accessories

Getting started | Pump basics

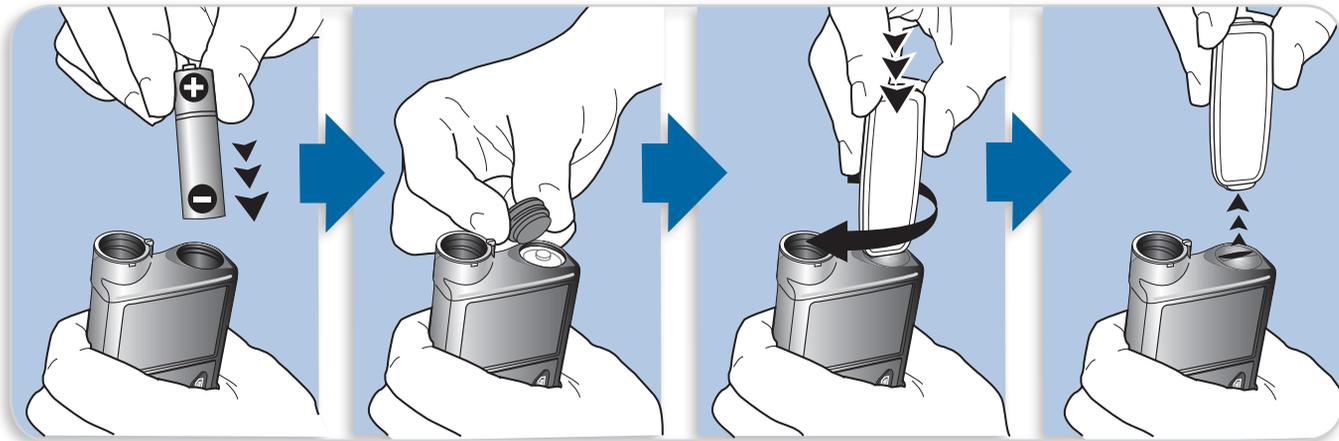


1 Place the battery into the battery compartment with the negative (flat) end going in first.

2 Place the battery cap onto the pump. Use the edge of the pump clip to turn the cap to the right (clockwise) and tighten until the slot is horizontal to the pump. See the following image.



CAUTION: Do not undertighten or overtighten the battery cap. Overtightening the battery cap can cause damage to your pump case. Undertightening the battery cap will prevent the pump from recognizing the new battery. Turn the battery cap clockwise until the cap is aligned horizontally with the pump case, as shown in the example to the right.

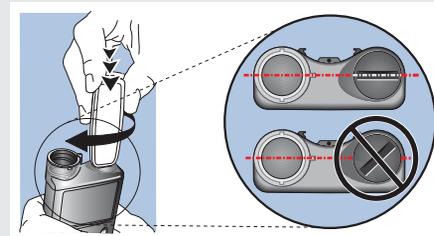

Section 4: Startup Wizard



The pump will power on and Startup Wizard will begin.



Note: Always look for the item on the screen that is highlighted in yellow. This is the item that can be selected. Press the and buttons to highlight the item you want to choose and press the button to select it.



Select your language.



Select **12 Hour** (AM/PM) or press to select **24 Hour** and press . *This example uses 12 Hour.*



The hour will be flashing. Press or to the correct hour and press .

The minutes will be flashing. Press or to the correct minutes and press .

If the 12-hour mode is selected, the AM/PM will be flashing. Press or if needed and press .

Select **Next**.




Select **Year**. Press to the correct year and press . Select **Month**. Press or to the correct month and press .

Select **Day**. Press or to the correct day and press .

Select **Next**.



Wait a moment.

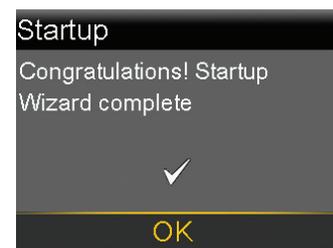

Select **OK**.



Note: To scroll faster, press and hold the or button. Once you reach the correct value or item, press to select.

Getting started | Home screen

Section 5: Home screen

You are now on the Home screen. The Home screen is your starting point. The following information is displayed on the Home screen.

Status icons: provides a quick look at the status of the pump.



Current time

BG reading: displays a BG taken in the last 12 minutes.

Active insulin: displays any insulin still active from a previous bolus.

Status icons

The Status icons can provide a quick look about the status of the pump. When using your pump, you will see the following icons:

Battery icon:

- The color and fill of the battery icon indicate the charge level of your pump battery.
- When your battery is full, the icon is solid green .
- As your battery life is used, the icon changes from solid green in the following order .
- When your battery is low, the icon has a single red bar . When your battery needs to be replaced immediately, the icon is solid black with a red outline .

Reservoir icon:

-  Approximately 85%–100% of the reservoir remains.
-  Approximately 71%–84% of the reservoir remains.
-  Approximately 57%–70% of the reservoir remains.
-  Approximately 43%–56% of the reservoir remains.
-  Approximately 29%–42% of the reservoir remains.
-  Approximately 15%–28% of the reservoir remains.
-  Approximately 1%–14% of the reservoir remains.
-  The reservoir remaining amount is unknown.



Audio icon: Shows the audio mode that you are using: audio , vibrate , or audio and vibrate .



Note: There will be times when you will need additional status information than is indicated by the status icons. For instance, the Reservoir icon may indicate your reservoir is getting low on insulin, but you may need to know exactly how many units are left. Additional information can be found in the status screens, see *Menu options on page 10*.

Unlocking the pump

After the Backlight has been off for a few minutes, the pump goes into Sleep mode and the pump is locked. When you wake up your pump from Sleep mode, you must unlock your pump before navigating to the menu. Press the button that is highlighted to unlock the pump. This confirms you are reading the screen and the button presses are not accidental.



If you press an incorrect button, the screen prompts you to try again.

If you press the Back  button, you will be taken to the current Home screen.

You can press and hold  if you wish to put the pump into Sleep mode and keep it locked when you are not using it. Doing this can also help save battery life.

Backlight

When you are not pressing buttons on your pump, you will notice that the Backlight will soon turn off. The pump is still on, it is just saving battery life. You can simply press any button to make the screen reappear.

Keeping the screen on longer...

Margaret noticed when she was not pressing buttons on her pump, the screen would turn dark. This happens to save battery life. She soon learned she could simply press any button to turn the screen back on.

Helpful hint: If the pump screen is going dark too quickly, the Backlight setting can be changed. To learn how to do this, see *Display Options on page 15*.




Getting started | Menu

Section 6: Menu

There are seven items on the main menu. Each menu item contains the features and functions that pertain to that menu item.

From the Home screen, press  to go to the menu.

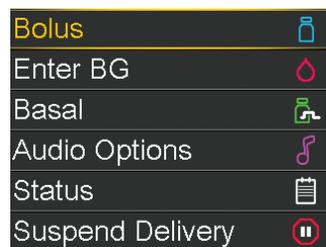

scroll bar

When a screen or a menu has more than six lines the scroll bar appears on the right side of the screen. Press  to view the additional items.

Menu options

Here you see a brief summary of the information found within each menu item.

| | |
|----------------------|--|
| Bolus | Lets you to choose between Bolus Wizard, Manual Bolus, or Preset Bolus. You can also access your Delivery Settings from here. |
| Enter BG | You can manually enter a BG reading from this screen. |
| Basal | Lets you switch to a Temp Basal or a Preset Temp basal rate, or change to a different Basal Pattern. You can also access your Delivery Settings from here. |
| Audio Options | Lets you choose Audio, Vibrate, or both to inform you of alerts and notifications. You can also change the volume here and go to the Alert Silence screen. |

| | |
|-------------------------|---|
| Status | Status screens let you view information about Auto Mode readiness; notifications you have received in the last 24 hours; Quick Status, including your last bolus, last BG entry, current basal rate, and estimated reservoir volume and battery status; pump status including estimated reservoir volume, when it was started, time left, and pump serial number; sensor status, including last calibration and next calibration due; and settings review, which includes your current pump settings. |
| Suspend Delivery | Lets you stop all insulin delivery. This is commonly used when disconnecting to swim or bathe. |
| Options | Lets you select, History, Reservoir & Tubing, Delivery Settings, Event Markers, Reminders, and access the Utilities menu. |
| Utilities | Lets you select Airplane Mode, Display Options, Time & Date, Remote Bolus, Block, Self Test, Manage Settings, Sensor Demo, Device Options, and Language. |




Note: You will not be using all of these options right away. We will focus on the ones that you will need to get started.

The Menu...

When Lisa first started on her pump, she did not know if she could ever learn how to use all the features the pump had available. But, she just focused on the basics first, and then she started learning the additional features that she found helped her the most.

Helpful hint: Take some time to get comfortable with the basics first. Then learning the additional features will be much easier and more fun to do.

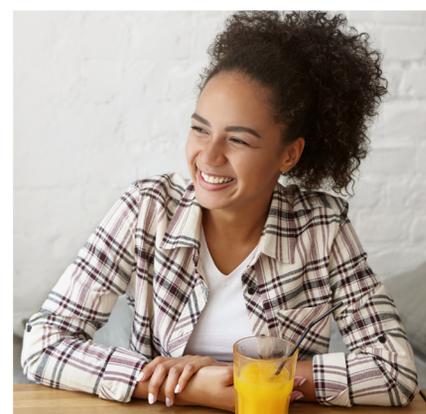

Getting started | Menu

MAIN MENU



Bolus

- Bolus Wizard
- Manual Bolus
- Preset Bolus
- Delivery Settings

Basal

- Temp Basal
- Preset Temp
- Basal Patterns
- Delivery Settings


Manual Mode

- Bolus
- Enter BG
- Basal
- Audio Options
- Status
- Suspend Delivery
- Options

Options

- SmartGuard** *(not available for use at this point in time)*
 - ▶ Auto Mode
 - ▶ Auto Mode (On/Off)
 - ▶ Auto Mode BG Alert (On/Off)
 - ▶ High Setup
 - ▶ Alert before high (On/Off)
 - ▶ Time before high
 - ▶ Alert on high (On/Off)
 - ▶ Rise Alert (On/Off)
 - ▶ Rise Limit
 - ▶ Low Setup
 - ▶ Alert before Low (On/Off)
 - ▶ Alert on Low (On/Off)
 - ▶ Suspend before Low (On/Off)
 - ▶ Suspend on Low (On/Off)
 - ▶ Resume basal alert (On/Off)
 - ▶ Snooze
 - ▶ High Snooze
 - ▶ Low Snooze
- History**
 - ▶ Summary
 - ▶ Daily History
 - ▶ Alarm History
 - ▶ Sensor Glucose Review
 - ▶ ISIG History
- Reservoir & Tubing**
 - ▶ New Reservoir
 - ▶ Fill Cannula
- Delivery Settings**
 - ▶ Bolus Estimate Setup
 - ▶ Carb Ratio
 - ▶ Bolus Wizard (On/Off)
 - ▶ Insulin Sensitivity Factor
 - ▶ BG Target
 - ▶ Active insulin time
 - ▶ Basal Pattern Setup
 - ▶ Preset Temp Setup
 - ▶ Preset Bolus Setup
 - ▶ Dual/Square Wave
 - ▶ Bolus Increment
 - ▶ Max Basal/Bolus
 - ▶ Easy Bolus
 - ▶ Auto Suspend
 - ▶ Bolus Speed
- Event Markers**
 - ▶ BG
 - ▶ Injection
 - ▶ Food
 - ▶ Exercise
 - ▶ Other
- Reminders**
 - ▶ Personal
 - ▶ Bolus BG Check
 - ▶ Missed Food Bolus
 - ▶ Low Reservoir
 - ▶ Set Change
- ▶ **Calibration** *(not available for use at this point in time)*
- Utilities**
 - ▶ **Sensor Settings** *(not available for use at this point in time)*
 - ▶ Sensor (On/Off)
 - ▶ Sensor Connections
 - ▶ Calibrate Sensor
 - ▶ **Airplane Mode**
 - ▶ **Display Options**
 - ▶ Brightness
 - ▶ Backlight
 - ▶ **Time & Date**
 - ▶ **Remote Bolus**
 - ▶ **Block**
 - ▶ **Self Test**
 - ▶ **Manage Settings**
 - ▶ Save Settings
 - ▶ Restore Settings
 - ▶ Clear All Settings
 - ▶ Clear Active Insulin
 - ▶ Settings History
 - ▶ **Sensor Demo**
 - ▶ **Device Options**
 - ▶ Manage Devices
 - ▶ Connect Device
 - ▶ **Language**

MAIN MENU

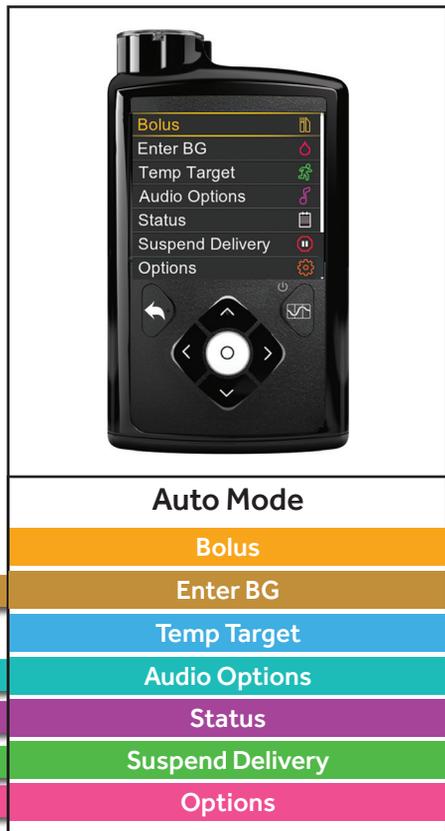

Bolus 

BG
Carbs

Enter BG 

BG Entry

Temp Target 

Duration
Cancel Temp Target

Audio Options 

Alert Silence Options

- ▶ High Alerts Only
- ▶ High & Low Alerts
- ▶ All Sensor Alerts
- ▶ Duration

Audio (On/Off)
Vibrate (On/Off)
Volume (-/+)

Status 

Auto Mode Readiness
(not available for use at this point in time)

Notifications
Quick Status
Pump
Sensor *(not available for use at this point in time)*
Settings Review

Suspend Delivery 

Section 7: Main menu items—a closer look

Now you are ready to set some basic features found within the Menu.

Audio Options


You will use Audio Options to set the pump to beep (Audio), vibrate (Vibrate), or beep and vibrate (Audio and Vibrate). If you choose Audio or Audio and Vibrate, you can also increase or decrease the Volume.

Let's practice:

- 1) Press  to open the Menu.
- 2) Press  to **Audio Options** and press .
- 3) Press  to the option that you prefer and press .
If you choose Audio, you are able to adjust the volume.
- 4) Press  to **Volume** and press .
- 5) Press  or  to the desired volume and press .
- 6) Select **Save**.



Note: You can have both Audio and Vibrate on at the same time.

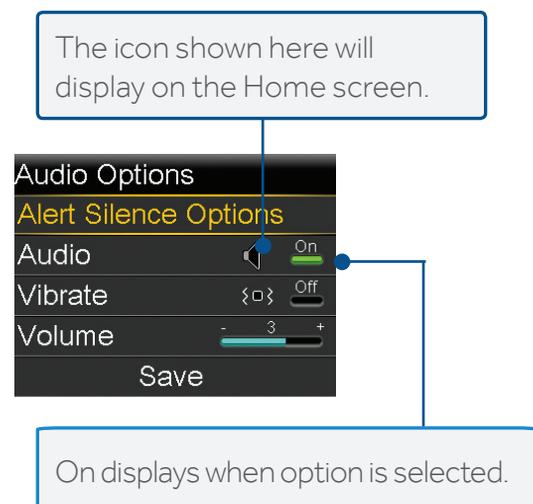



Getting started | Main menu items

Display Options

Display Options allows you to choose the brightness of your pump screen. This is also where you go to change the amount of time your pump stays on before it goes into Power Save mode.



Let's practice:

- 1) Press to open the Menu.
 - 2) Press to **Options** and press .
 - 3) Press to **Utilities** and press .
 - 4) Press to **Display Options** and press .
- If you want to adjust the screen brightness:
- 5) Select **Brightness**.
 - 6) Press or to the setting you prefer and press .



Note: The Auto setting automatically adjusts the screen brightness to match your current environment. Your pump arrives set to Auto.

To adjust the backlight:

- 7) Select **Backlight**.
- 8) Press or to the setting you prefer and press .
- 9) Select **Save**.




Note: How you adjust these settings can affect battery life. Increasing the Backlight time will decrease the life of your battery.



Section 8: Basal Patterns


Remember, your body needs insulin so glucose can be moved into your cells providing energy for your body. Insulin is needed 24 hours a day, even between meals and during the night. This is called basal insulin. The pump supplies basal insulin by delivering small amounts throughout each hour, every hour of the day and night. This allows for insulin to be increased and decreased to adjust for your body's needs.

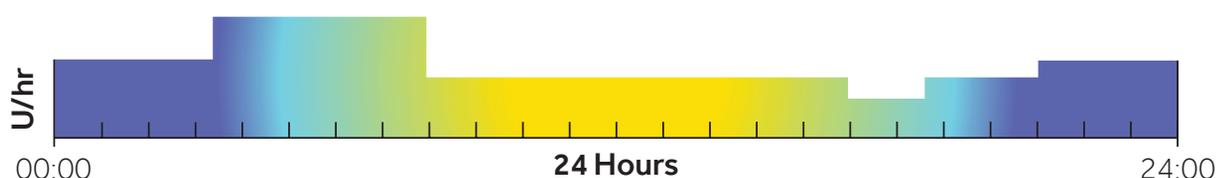

Basal insulin amounts must be programmed into your pump. This is done by setting a basal pattern. A basal pattern consists of one or more basal rates being delivered over the course of 24 hours.

Before her pump...

Lynn always had to remember to take her shot of long-acting insulin at bedtime. Taking it at the same time every night like her doctor asked her to was difficult. She is in college and some nights she would go to bed early, others she would be at the library until late studying. Now that her doctor has prescribed a pump, she does not have to worry about taking a shot. She is getting her basal insulin automatically 24 hours a day.

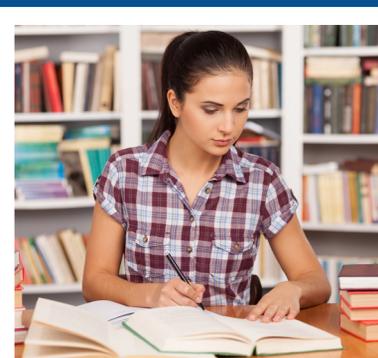

Basal Pattern Setup—one basal rate

Your healthcare professional will calculate the hourly basal rate or rates that are best for you to use when you start on your pump. You may simply start with a basal pattern that has only one basal rate. The pump will deliver that exact basal amount evenly over each hour, 24 hours a day.

For example, if your starting basal rate is 1.0 unit, your pump would deliver one unit of insulin throughout each hour. This means you would receive a total of 24 units of basal insulin every 24 hours. To set Basal Patterns, go to **Delivery Settings**.

- 1) Press to open the Menu.
- 2) Press to highlight **Basal**. Press .
- 3) Press to highlight **Delivery Settings**. Press .



Note: You can also access Delivery Settings from the Options menu.





WARNING: The following are some examples of basal rates for you to practice entering while learning how to use your pump. You will need to work with your healthcare professional to get your personal basal rates. Do not use these practice basal rates for your therapy. Attempting to use these settings in your pump could result in the delivery of too little or too much insulin, which can cause hyperglycaemia or hypoglycaemia.



Let's practice: setting a Basal Pattern that has only one basal rate


Let's set a basal pattern with a basal rate of 0.750 U/hr from 00:00-24:00.

- 1) Press  to open the Menu.
- 2) Press  to **Basal** and press .
- 3) Press  to **Delivery Settings** and press .
- 4) Press  to **Basal Pattern Setup** and press .
- 5) Select **Basal 1**.
- 6) Select **Options**.

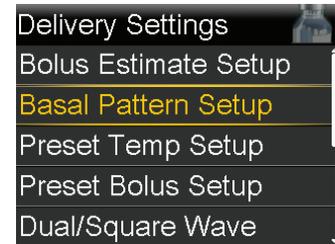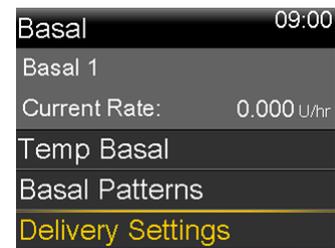

Getting started | Basal Patterns

7) Select **Edit**.

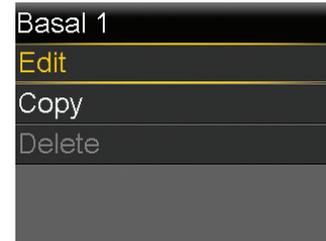

8) Press on the time segment. The **End** time will be flashing.



9) Since you have only one basal rate, you do not need to change the **End** time. Press on the 24:00.

10) Press to enter 0.750 and press .



11) Select **Done**.



12) Verify that the basal pattern is entered correctly. Make sure the **24 hr Total** is accurate.



13) If no changes need to be made, select **Save**.

If changes need to be made, press to return to the Edit Basal 1 screen.


14) Press and to edit the time segment.

15) Select **Done**.

16) When finished, select **Save**.

This basal rate amount entered, 0.750 units per hour in this example, will automatically be delivered throughout each hour continuously from one day to the next.

Note: This basal pattern delivers 18 U over 24 hours.

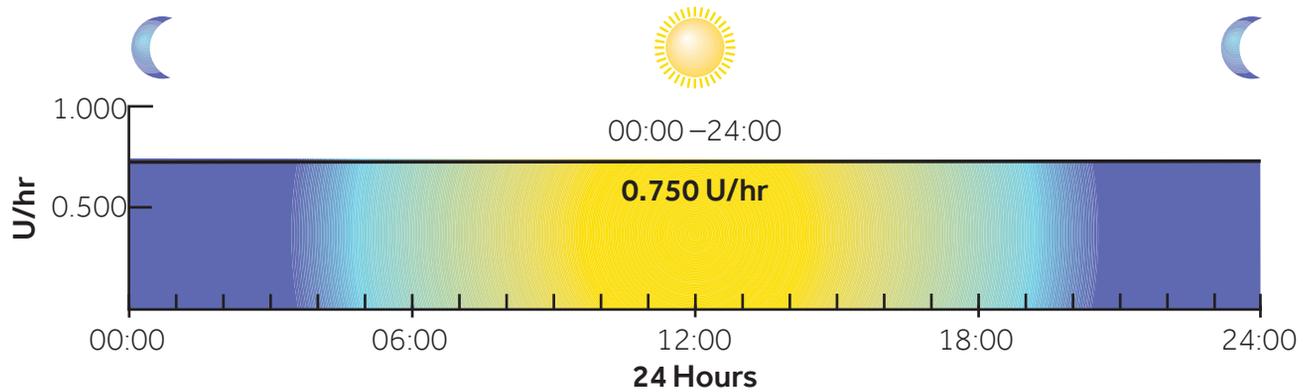

Basal Pattern Setup—changing a basal rate

When you check your blood glucose (BG) as instructed, the BG readings will help you and your healthcare professional determine if your basal pattern needs to be changed. If your glucose levels are running too high or too low, this basal amount may need to be changed.

Let's practice: changing a basal rate

Change the **Basal 1** basal rate from 0.750 to 0.900 U/hr.

- 1) Press to go to the Menu.
- 2) Press to **Basal** and press .
- 3) Press to **Delivery Settings** and press .
- 4) Press to **Basal Pattern Setup** and press .
- 5) Select **Basal 1**.
- 6) Select **Options**.
- 7) Select **Edit**.
- 8) Press on the time segment.
- 9) Press to **Rate** and do not select it.
- 10) Press to change 0.750 to 0.900 and press .
- 11) Select **Done**.

| Edit Basal 1 | | |
|--------------|-------|-------|
| Start | End | U/hr |
| 00:00 | 24:00 | 0.750 |
| Done | | |



| Edit Basal 1 | | |
|--------------|-------|-------|
| Start | End | U/hr |
| 00:00 | 24:00 | 0.900 |
| Done | | |

Getting started | Basal Patterns

- 12) Verify that **Basal 1** is entered correctly.
- 13) Select **Save**.

| Basal 1 | | |
|-------------|-------|-------|
| Start | End | U/hr |
| 00:00 | 24:00 | 0.900 |
| Save | | |

Basal Pattern Setup—multiple basal rates

After you start using your insulin pump, your glucose reading will help you and your healthcare professional determine if your basal pattern needs to be changed. Not only might you need to increase or decrease your current rate, you may also need to add basal rates to give you different amounts of basal insulin during certain times of the day or night.

Having more than one basal rate...

When Jessica was taking shots, her BG readings were always high in the morning. If she increased her nighttime insulin, then she would have low BGs later in the day. Now that she has her pump, it is set to deliver more insulin in the early morning so her BG values are not high when she wakes up, and less insulin later in the day when she needs a lower dosage.


Helpful hint: Most people need more than one basal rate to get the best control with their pump. Work with your healthcare professional to get your basal rates adjusted correctly when you start on pump therapy.



Getting started | Basal Patterns

In this example, a healthcare professional reviewed the BG readings and has determined that one basal rate works well for part of the day, but the basal rate needs to be lowered to 0.650 units per hour between the hours of 08:00 and 18:00.

The new basal pattern will look like this:

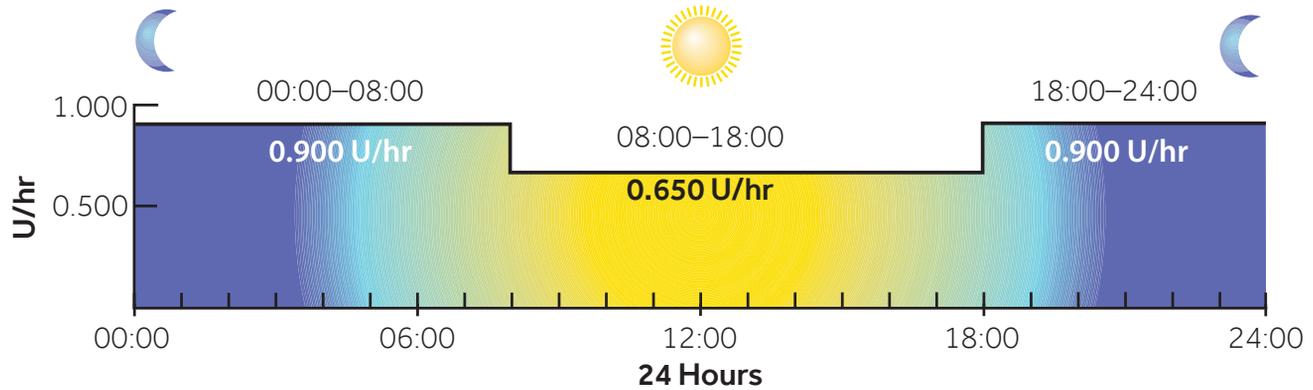

Now, let's make the changes to the basal pattern.

Let's practice: setting multiple basal rates

- 1) Press to go to the Menu.
- 2) Press to select **Basal** and press .
- 3) Press to **Delivery Settings** and press .
- 4) Press to **Basal Pattern Setup** and press .
- 5) Select **Basal 1**.
- 6) Select **Options**.
- 7) Select **Edit**.
- 8) Press on the time segment.

| Start | End | U/hr |
|-------|-------|-------|
| 00:00 | 24:00 | 0.900 |
| Done | | |

The 0.900 basal rate will now need to end at 08:00 since this is the time that your basal rate needs to decrease.

- 9) Press to 08:00 and press .
- 10) Press again as this basal rate will stay the same.

| Start | End | U/hr |
|-------|-------|-------|
| 00:00 | 08:00 | 0.900 |
| 08:00 | 08:30 | --- |
| Done | | |

Getting started | Basal Patterns

You can see you are automatically asked to enter the end time of the second basal rate. This basal rate will need to end at 18:00 and will need to be changed to 0.650.

- 11) Press  to change the **End** time.
- 12) Press  to 18:00 and press .
- 13) Press  to 0.650 and press .

You can now enter the next end time. You will need to enter 24:00 to complete the full 24 hours.

- 14) Press  to change the **End** time.
- 15) Press  to 24:00 and press .
- 16) Press  to 0.900 and press .
- 17) Select **Done**.

- 18) Verify that **Basal 1** is entered correctly. Press  to view all the basal rates.
- 19) Select **Save**.

| Edit Basal 1 | | |
|--------------|-------|-------|
| Start | End | U/hr |
| 00:00 | 08:00 | 0.900 |
| 08:00 | 18:00 | 0.650 |
| 18:00 | 18:30 | --- |
| Done | | |

| Edit Basal 1 | | |
|--------------|-------|-------|
| Start | End | U/hr |
| 00:00 | 08:00 | 0.900 |
| 08:00 | 18:00 | 0.650 |
| 18:00 | 24:00 | 0.900 |
| Done | | |

| Basal 1 | | |
|---------------------|-------|-------|
| 24 hr Total: 19.1 U | | |
| Start | End | U/hr |
| 00:00 | 08:00 | 0.900 |
| 08:00 | 18:00 | 0.650 |
| Save | | |

Let's practice: changing multiple basal rates

Now change the 08:00 to 18:00 basal rate to 08:00 to 17:30 and change to 0.700 U/hr.

- 1) Press  to go to the Menu.
- 2) Press  to select **Basal** and press .
- 3) Press  to **Delivery Settings** and press .
- 4) Press  to **Basal Pattern Setup** and press .
- 5) Select **Basal 1**.
- 6) Select **Options**.
- 7) Select **Edit**.
- 8) Press  to the 08:00 to 18:00 time segment and press .
- 9) Press  to 17:30 and press .
- 10) Press  to 0.700 and press . Notice the start time of the 3rd time segment changed to 17:30.
- 11) Press  to change the **End** time.
- 12) Press  to 24:00 and press .
- 13) Press  to 0.900 and press .
- 14) Select **Done**.
- 15) Verify that the **Basal 1** is entered correctly. Press  to view all the basal rates.
- 16) Select **Save**.

| Edit Basal 1 | | |
|--------------|-------|-------|
| Start | End | U/hr |
| 00:00 | 08:00 | 0.900 |
| 08:00 | 18:00 | 0.650 |
| 18:00 | 24:00 | 0.900 |
| Done | | |



| Edit Basal 1 | | |
|--------------|-------|-------|
| Start | End | U/hr |
| 00:00 | 08:00 | 0.900 |
| 08:00 | 17:30 | 0.700 |
| 17:30 | 24:00 | 0.900 |
| Done | | |

| Basal 1 | | |
|---------------------|-------|-------|
| 24 hr Total: 19.7 U | | |
| Start | End | U/hr |
| 00:00 | 08:00 | 0.900 |
| 08:00 | 17:30 | 0.700 |
| Save | | |

Basal Pattern Setup—removing basal rates

There may be times when you have basal rates entered that need to be removed. This is done by simply changing the end time of the last basal rate that you need to 24:00.

Let's practice: removing basal rates

- 1) Press  to go to the Menu.
- 2) Press  to **Basal** and press .
- 3) Press  to **Delivery Settings** and press .
- 4) Press  to **Basal Pattern Setup** and press .
- 5) Select **Basal 1**.
- 6) Select **Options**.
- 7) Select **Edit**.
- 8) Press  on the 00:00 to 08:00 time segment.
- 9) Press  to 24:00 and press .
- 10) Press  again as this basal rate will stay the same. Notice that all other basal rates have been removed.
- 11) Select **Done**.
- 12) Verify that **Basal 1** is entered correctly.
- 13) Select **Save**.

| Edit Basal 1 | | |
|--------------|-------|-------|
| Start | End | U/hr |
| 00:00 | 08:00 | 0.900 |
| 08:00 | 17:30 | 0.700 |
| 17:30 | 24:00 | 0.900 |
| Done | | |



| Edit Basal 1 | | |
|--------------|-------|-------|
| Start | End | U/hr |
| 00:00 | 24:00 | 0.900 |
| Done | | |

| Basal 1 | | |
|---------------------|-------|-------|
| 24 hr Total: 21.6 U | | |
| Start | End | U/hr |
| 00:00 | 24:00 | 0.900 |
| Save | | |

Suspend Delivery

Remember that your pump is delivering basal insulin throughout every hour of the day. Although you should never stop this insulin delivery for more than an hour or so, there will be times when you will want to manually suspend, or stop delivery, and disconnect from your pump. This is done using the manual Suspend Delivery feature. Using Suspend Delivery stops all insulin delivery. The most common reasons to manually suspend delivery might include bathing and water activities. Infusion sets are designed so you can easily disconnect from your pump and leave it in a safe place. Talk with your healthcare professional about a plan including BG checks and possible correction boluses when disconnecting and reconnecting your pump.

Suspending the pump...



Danielle prefers not to wear her pump when she is swimming, so she disconnects it. She always manually suspends her pump so that insulin is not delivered while the pump is not attached to her.



Helpful hint: While the pump is suspended, it will beep, vibrate, or beep and vibrate every 15 minutes to remind you insulin delivery is suspended unless a button is pressed.


Let's practice: Placing the pump in manual suspend

- 1) Press  to open the Menu.
- 2) Press  to highlight Suspend Delivery.
- 3) Select **Suspend Delivery**.
- 4) Press  and select **Yes** to suspend delivery.

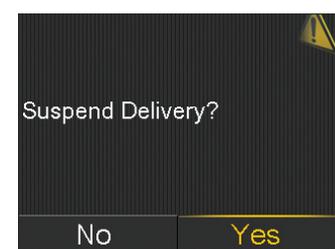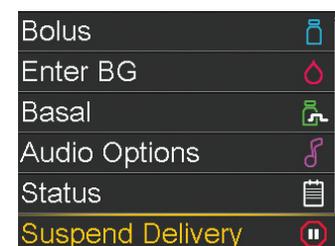


Getting started | Basal Patterns

A confirmation screen appears.

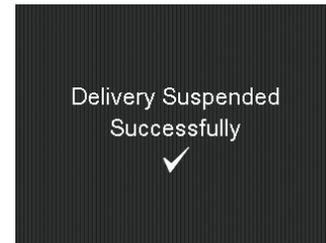

Notice that the Home screen has changed. The pump will beep, vibrate, or beep and vibrate every 15 minutes while the pump is manually suspended unless a button is pressed.

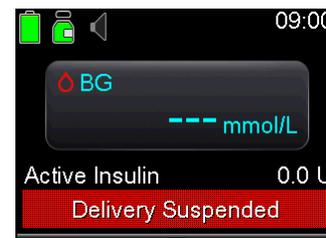


WARNING: When delivery is resumed, basal insulin will begin to deliver again. The pump will not deliver any of the basal insulin you missed while the pump was suspended.

If you manually suspend delivery while a bolus is delivering, the bolus delivery will stop. When you resume delivery, the remainder of the bolus will not be delivered.




Let's practice: Resuming basal insulin delivery

1) Press  to open the Menu.

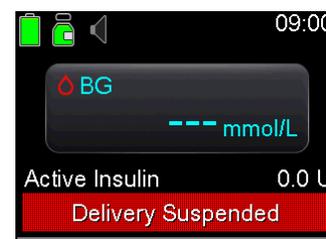


2) Select **Resume Delivery**.

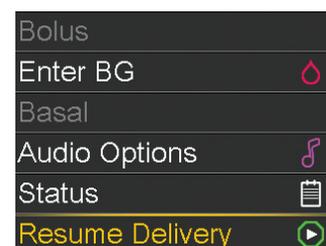

Getting started | Basal Patterns

- 3) Press  and select **Yes** to resume insulin delivery.

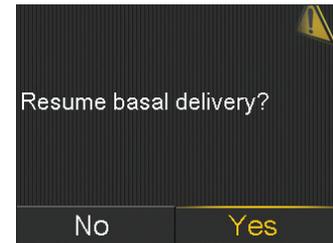

A confirmation screen appears.



The Home screen appears.



Section 9: Giving boluses

A bolus is given for two reasons: to cover food that contains carbohydrate or to correct glucose levels that are above your target range. Giving a bolus will be one of the most common things you do with your pump. Instead of having to take shots at meals, or between meals if your glucose is too high, you can program your pump to give the insulin. When using the pump, you are able to give precise bolus amounts.

Giving a bolus...

Susie finds it easier to give herself a bolus on her pump than it was to give an injection at her meals. When she went out to eat, she would sometimes forget to take her insulin along. Now it is always with her.



Giving a manual bolus

When giving a manual bolus, you simply enter the amount of bolus insulin that you think you need for the carbohydrates you are eating, or to lower your BG if it is high.



WARNING: Make sure you are NOT connected to the pump while you are giving practice boluses.

- 1) Press  to open the Menu.
- 2) Select **Bolus**.
- 3) Press  to 1.0 u and press .
- 4) Select **Deliver Bolus**.


| | |
|----------------|--------------|
| Manual Bolus | 09:00 |
| BG | --- mmol/L |
| Active Insulin | 0.0 U |
| Bolus | 1.0 U |
| Deliver Bolus | |

| | |
|----------------------|--------------|
| Manual Bolus | 09:00 |
| BG | --- mmol/L |
| Active Insulin | 0.0 U |
| Bolus | 1.0 U |
| Deliver Bolus | |


- Confirmation that the Bolus has started will appear.



The Home screen will show the amount as it is being delivered. Once the bolus has finished delivering, the pump will return to the normal Home screen.

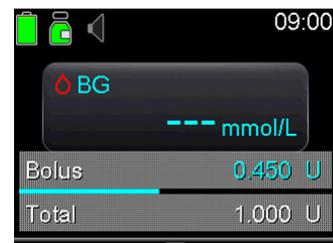


Notice there is **Active Insulin** now displayed. Active insulin is insulin from boluses that is still working to lower blood glucose levels. Each time you give a bolus, it is added to the active insulin amount. As time passes, the amount will decrease. You will learn more about active insulin during your training.

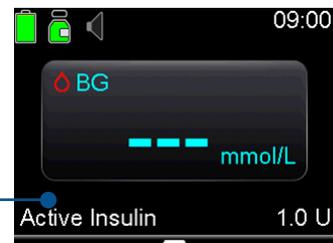

Stopping a bolus that you have started

There may be times when you need to stop your bolus. Perhaps you realised you entered the wrong amount, or you get a phone call and cannot eat right now as planned. Go to the Main Menu to find the **Stop Bolus** option.

- Press to open the Menu.
- Select **Stop Bolus**.
- Press and select **Yes**.

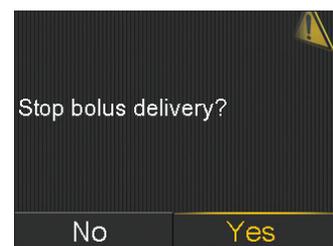

Getting started | Giving boluses

- 4) Review the **Bolus Stopped** screen to see how much of the bolus was delivered.
- 5) Select **Done**.



Note: The **Bolus Stopped** screen will show you how much of the bolus insulin was delivered before it was actually stopped.



Stopping a Bolus...

Karen gives a bolus for lunch, but before she can begin eating, the phone rings. It's her cousin calling long distance, so Karen knows this phone call will take a while. She decides to wait to eat until after the call so she stops the bolus.

Helpful hint: Always check the Bolus Stopped screen to see how much insulin you received before the bolus was stopped. Depending on the amount, you may decide you need to eat something so you do not experience a low blood glucose.



Let's practice: Stopping a bolus

Give a manual bolus of 1.5 units and stop the bolus once it has started to deliver.

- 1) Press  to open the Menu.
- 2) Select **Bolus**.
- 3) Press  to 1.5 u and press .
- 4) Select **Deliver Bolus**.
- 5) Press  to open the menu, then select **Stop Bolus**.
- 6) Press  and select **Yes** to stop delivery.
- 7) Review the **Bolus Stopped** screen. How much of the bolus was delivered?
- 8) Select **Done**.

Bolus Wizard

Calculating how much bolus insulin to give can be challenging. When using the Bolus Wizard feature, you will enter your current BG reading along with the amount of carbs you are about to eat. Once you do this, the Bolus Wizard feature uses the individual settings provided by your healthcare professional to calculate your bolus amount.

By counting carbs and using the Bolus Wizard feature, you are able to give the right amount of insulin for your food and correction bolus. This can help to keep your glucose levels better controlled.



WARNING: The following are some examples of Bolus Wizard settings for you to practice entering while learning how to use your pump. You will need to work with your healthcare provider to get your personal Bolus Wizard settings. Do not use these practice Bolus Wizard settings for your therapy. Attempting to use these settings in your pump could result in the delivery of too little or too much insulin, which can cause hyperglycaemia or hypoglycaemia.



Bolus Wizard Setup

To use the Bolus Wizard feature, you must first enter your personal settings from your healthcare professional. You will need your Carb Ratio, Sensitivity Factor, BG Targets, and your Active Insulin Time to complete the setup. If you do not have your personal settings yet, you may practice with the practice settings in the examples below. Be sure your personal settings are entered before actually using the Bolus Wizard feature for your therapy.



Let's practice: entering Bolus Wizard settings

- 1) Press .
- 2) Select **Options**.
- 3) Select **Delivery Settings**.
- 4) Select **Bolus Estimate Setup**.
- 5) Select **Bolus Wizard** to turn it on.

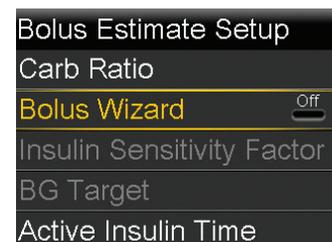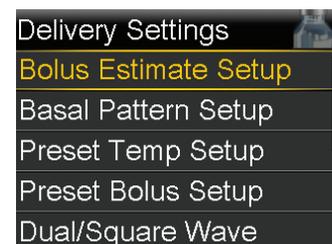

Getting started | Giving boluses

- 6) Press to continue reading text.
- 7) Select **Next**.

- 8) Review the description of Carb Ratio and select **Next**.

- 9) Press on the time segment.
- 10) If you have only one Carb Ratio, press .




If you have more than one Carb Ratio, press or to enter the time that your Carb Ratio ends and the second begins and press .

- 11) Press or to enter the **g/U** of your Carb Ratio and press .

If you have more than one Carb Ratio, continue by entering your time segments and Carb Ratios until all are entered.

This example shows only one Carb Ratio of 15. Enter this practice Carb Ratio, or if you know your personal Carb Ratio, enter it now.

- 12) Select **Next**.
- 13) Review the description of Sensitivity Factor and select **Next**.

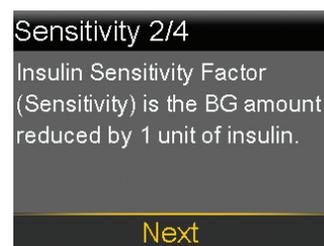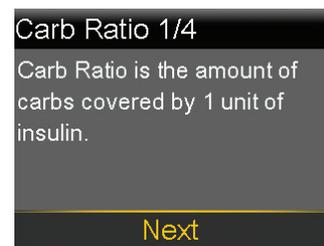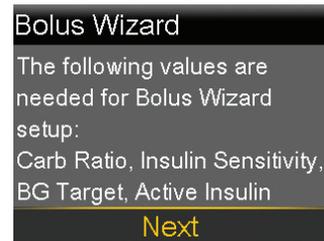

14) Press  on the time segment.

15) If you have only one Sensitivity Factor, press .

If you have more than one Sensitivity Factor, press  or  to enter the time that your Sensitivity Factor ends and the second begins and press .

| Edit Sensitivity 2/4 | | |
|----------------------|-------|--------------|
| Start | End | mmol/L per U |
| 00:00 | 24:00 | --- |

16) Press  or  to enter the **mmol/L per U** of your Sensitivity Factor and press .

If you have more than one Sensitivity Factor, continue by entering your time segments and Sensitivity Factors until all are entered.

This example shows only one Sensitivity Factor of 2.8. Enter this practice Sensitivity Factor, or if you know your personal Sensitivity Factor, enter it now.

| Edit Sensitivity 2/4 | | |
|----------------------|-------|--------------|
| Start | End | mmol/L per U |
| 00:00 | 24:00 | 2.8 |
| Next | | |

17) Select **Next**.

18) Review the description of BG Target and select **Next**.

| BG Target 3/4 |
|---|
| BG Target is the value your blood glucose level will be corrected to. |
| Next |

19) Press  on the time segment.

20) If you have only one BG Target range, press .

If you have more than one BG Target range, press  or  to enter the time that your BG Target range ends and the second begins and press .

| Edit BG Target 3/4 | | |
|--------------------|-------|----------------|
| Start | End | Lo-Hi (mmol/L) |
| 00:00 | 24:00 | --- -- |

Getting started | Giving boluses

- 21) Press or to enter the Lo target and press .
- 22) Press or to enter the Hi target and press .

If you have more than one BG Target Range, continue by entering your time segments and Lo and Hi targets until all are entered.

This example shows only one BG Target Range of 5.6-5.6. Enter this practice BG Target Range, or if you know your personal Bolus Wizard BG Target Range, enter it now.

- 23) Select **Next**.
- 24) Review the description of Active Insulin Time and select **Next**.





- 25) Select **Duration**.
- 26) Press or to enter the **Duration** of your Active Insulin Time and press .

This example shows an Active Insulin Time of 4:00 hours. Enter this practice Active Insulin Time, or if you know your personal Active Insulin Time, enter it now.

- 27) Select **Save**.

The Bolus Wizard setup is now complete.

Now that you have completed the initial setup, you can see that the individual settings are now accessible menu items. If you need to make a change to any of these settings, you can press down to the setting, select it, and make the necessary changes.

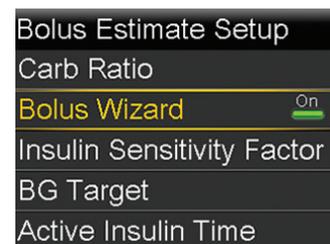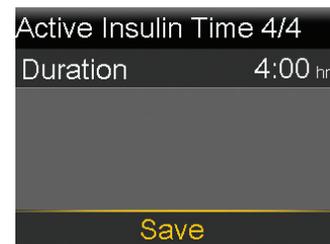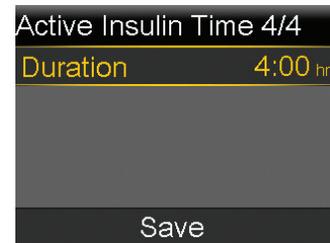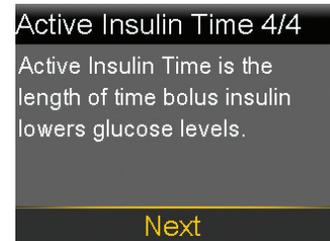

Using the Bolus Wizard feature

Before we start, let's take a look at the Bolus Wizard entry screen.

The screenshot shows the 'Bolus Wizard' screen with the following fields and callouts:

- Current BG from BG meter:** Points to the 'BG' field.
- Active insulin being subtracted from correction insulin because it is still lowering glucose levels:** Points to the 'Active Ins. adjust.' field.
- Number of grams of carbs you are eating:** Points to the 'Carbs' field.
- Correction insulin needed for BG above target, or insulin subtracted for BG below target:** Points to the 'Bolus' field.
- Amount of active insulin being deducted:** Points to the 'Active Ins. adjust.' field.
- Insulin needed for carbs:** Points to the 'Carbs' field.
- Total estimated bolus amount:** Points to the 'Bolus' field.


Let's practice: Food and correction bolus

Now you are ready to practice giving a bolus. This example shows giving a bolus for a BG and carbs. In this example we will use a BG value of 6.8 mmol/L and 35 grams of carbs.

- 1) Press .
- 2) Select **Bolus**.
- 3) Select **Bolus Wizard**.
- 4) Select **BG**.
- 5) Press  or  to enter the current BG, and press .

Active Ins. adjust. is the active insulin from previous boluses that is being adjusted (subtracted) from the correction dose.

- 6) Select **Carbs**.
- 7) Press  to enter the amount of carbs you are eating and press .
- 8) Select **Next**.

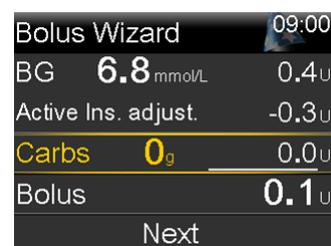


Getting started | Giving boluses

9) Select **Deliver Bolus**.



Note: The BG value entered appears on the Home screen and will remain here for 12 minutes.

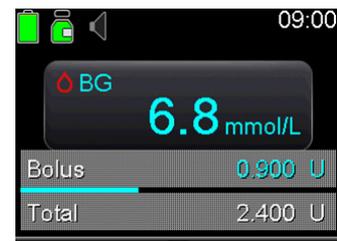

There may be times you enter either a BG value or carbs. For example, you would enter:

- only grams of carbs if you finished your meal, but are eating additional carbs
- only a BG value if you tested two hours after your meal to see if you needed a correction bolus

Let's practice: Food bolus with no BG

- 1) Press .
- 2) Select **Bolus**.
- 3) Select **Bolus Wizard**.
- 4) Press  to **Carbs** and press .
- 5) Press  to enter the amount of carbs you are eating and press .
- 6) Select **Next**.
- 7) Select **Deliver Bolus**.






Note: You will receive messages when you enter a BG below 3.9 mmol/L or above 13.9 mmol/L. These prompt you to take appropriate steps to treat as instructed by your healthcare professional. You will see an example in the next practice exercise.



Let's practice: Correction bolus with no food

- 1) Press .
- 2) Select **Bolus**.
- 3) Select **Bolus Wizard**.
- 4) If using the compatible meter, BG will be on screen. If not, select **BG**.
- 5) Press  or  to enter the current BG, and press .
- 6) Press  to **Next** and press .
- 7) The High BG message will appear. Read the text and press .
- 8) Continue reading the text and take appropriate action to prevent diabetic ketoacidosis (DKA).
- 9) Select **OK**.
- 10) Select **Deliver Bolus**

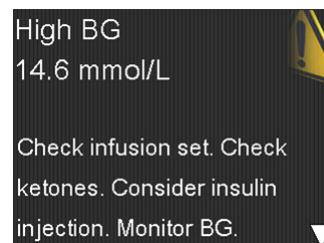

Getting started | Giving boluses




WARNING: Do not use the Bolus Wizard feature to calculate a bolus for a period of time after giving a manual injection of insulin by syringe or pen. Manual injections are not accounted for in the active insulin amount. Therefore, the Bolus Wizard feature could prompt you to deliver more insulin than needed. Too much insulin can cause hypoglycaemia. Consult with your healthcare professional for how long you need to wait after a manual injection of insulin before you can rely on the active insulin calculation made by the Bolus Wizard feature.


Status

There will be times when you need information about your pump status. For example, the status icon on your Home screen shows you if the insulin in your reservoir is getting low, but you may need to know exactly how many units are left. This information can be found in the Status screens.

- 1) From the Home screen, press .

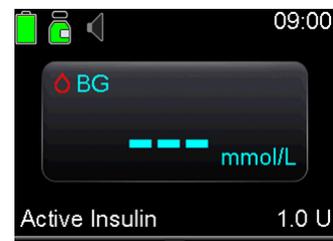

- 2) Press  to highlight **Status**.
- 3) Press  to select **Status**.
- 4) Press  to highlight the status item you wish to view and press .

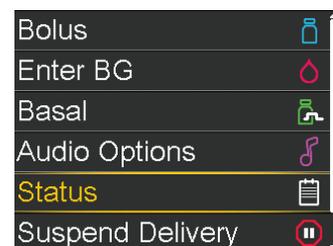

Here you can see the status information that can be found when you select each menu item:

| | |
|------------------------|--|
| Notifications | Shows the names and times of alarms, alerts, messages, and reminders that you have received over the past 24 hours. To see more alerts and alarms, go to History in Utilities. |
| Quick Status | Provides a current summary of pump information including the last bolus you delivered, the last BG entered, and your current basal rate. |
| Pump | Provides detailed information about your pump, including the date you last changed the reservoir, and the number of units left in it. |
| Settings Review | Displays the current settings you have programmed into your pump. |



Note: You can go back to the previous screen by pressing .

Checking last bolus

There may be times when you need to see the time or amount of the last bolus that was given. For example, you may not remember if you took a bolus at lunch and want to check to make sure. You can see the last bolus delivered in the **Quick Status** screen.



Let's practice: Checking last bolus

- 1) Press .
- 2) Press  to **Status** and press .
- 3) Press  to **Quick Status** and press .

The (N) behind the Last bolus amount means the bolus was delivered as a normal bolus. There are additional ways to give a bolus which you will learn about later in your training.

| | |
|---------------------|-------------|
| Quick Status | 09:00 |
| Last bolus | 2.800 U (N) |
| | 09:02 |
| | Jan 1 |
| Last BG | 14.6 mmol/L |
| | 09:03 |
| | Jan 1 |

Getting started | Giving boluses

Checking bolus history

You may also want to review the last several boluses that were delivered. For example, a parent might want to view the boluses their child gave throughout the day. You can see the last several boluses delivered in Daily History.



Let's practice: Checking bolus history

You can see the last several boluses you delivered in **Daily History**.

- 1) Press
- 2) Press to **Options** and press .
- 3) Press to **History** and press .
- 4) Press to **Daily History** and press .
- 5) Press on the day you would like to review.

| Daily History | 09:00 |
|-------------------|-------|
| Bolus (N) 1.000 U | 15:32 |
| Bolus (N) 1.500 U | 14:07 |
| Bolus (N) 2.000 U | 11:55 |
| ◀ Fri, Mar 30 ▶ | |




Note: You can press the and arrows to move from day to day. You can also see further details by pressing on any item listed.

Getting started | Using the compatible Ascensia BG meter

Section 10: Using the compatible Ascensia BG meter

The MiniMed 670G insulin pump can only wirelessly connect with a compatible Ascensia BG meter to receive remote BG readings. You can set up your insulin pump to automatically receive BG readings, which can be used with the Bolus Wizard feature and the Event Marker options.

Review the parts of your meter here:

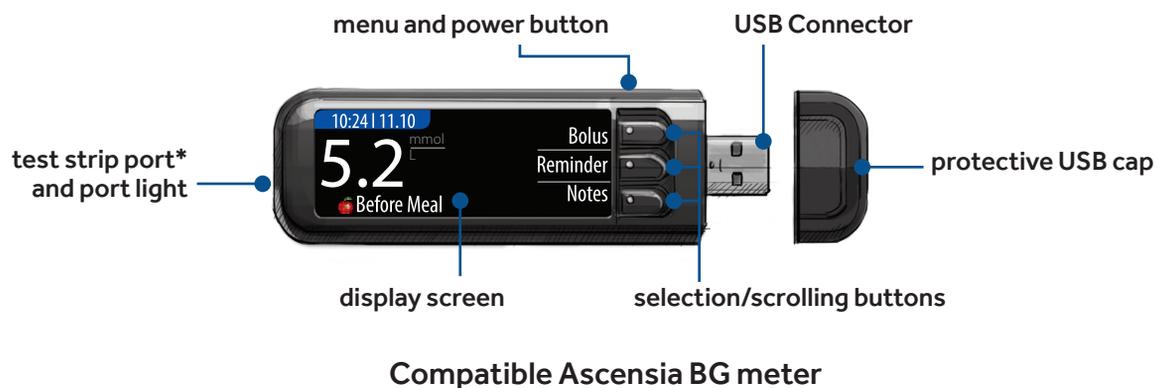

Charging your meter

Your meter has a permanent rechargeable battery. **It is important that you charge the meter prior to your in-person training.** To charge your meter:

- 1) Remove the cap to reveal the USB connector.
- 2) Plug the USB connector into the wall charger or a computer.

The computer must be ON and not in sleep, hibernate, or power save mode.



- 3) The meter will briefly display **Do Not Test—charging** and the test strip port light will flash. You cannot do a blood glucose test while the battery is charging.
- 4) When charging is complete, the test strip port light will turn off. You can then unplug the meter.

You will connect your pump and meter at your in-person training. Steps on how to connect your pump and meter are in *Training handouts on page 80*. For more information on using your meter, see the User Guide found in the meter box.

* *The compatible Ascensia BG meter only works with compatible Ascensia glucose testing strips.*

Getting started | Using the compatible Ascensia BG meter

Introduction to CareLink Personal software

CareLink Personal software is a web-based program that is provided free of charge by Medtronic. This software allows you to upload the data from your pump and glucose meter to a secure website and organise it into easy-to-read reports and charts. These reports provide an overview of how insulin, food intake, and exercise affect your glucose control.

Reviewing the data on these reports allows you and your healthcare professional to identify glucose patterns and trends so you can determine if any pump settings need to be adjusted.

You will need to set up your CareLink Personal account so you can upload your pump and meter every two to three days after you start using your pump. You and your healthcare professional will be able to review your information and adjust your pump settings as needed.

If you are not currently using CareLink Personal software, you can follow these steps to set up your account:

- 1) Go to <https://carelink.minimed.eu/>.
- 2) Select the **Sign Up Now** button.
- 3) Choose your country and language.
- 4) Read and **Accept** the Terms of Use and Privacy Statement.
- 5) Create a Username and Password and enter all required information.
- 6) Select **Submit**.

You will learn more about using CareLink software at your in-person training.

When uploading your information from your pump to CareLink software, you will use the meter as the communication device from the pump to your computer.

Using CareLink software...

Julia uploads her pump and meter information to CareLink Personal before each visit with her doctor. She has given him access to her reports so he can review them, saving a great deal of time during her office visit. Her doctor has the information he needs to make adjustments to her pump settings.





Section 11: Frequently asked questions

As with learning anything new, you typically have questions. Here is a list of commonly asked questions. You may wish to make a note of any additional questions you may have to ask your Certified Product Trainer.

Where should I wear my pump?

Where and how to wear the pump is a commonly asked question among new pump users. Most individuals find that wearing an insulin pump presents no problem and that it can be worn in a variety of ways. It typically takes only a day or two to find the ways that work best for you. Below are just a few ideas to help get you started.

- Use the clip that comes with your pump and clip it to a waist band or belt
- Place the pump (with or without the clip) into the pocket of your pants
- Keep it in your shirt pocket
- Slip it into your bra with the screen facing away from your skin
- Use the longer tubing lengths and place the pump in your sock

Where can I put the pump when I sleep?

- Clip it to the waist of your pajama pants
- Clip it onto your pajama top or in a pocket
- Place it next to you in the bed, under your pillow, or on the bedside table

Medtronic Diabetes offers accessories that can add to the convenience of wearing, protecting, and concealing your pump. Refer to the accessories catalog or to the accessories information found on our website at www.medtronic-diabetes.com.au

What about intimacy?

What to do with the pump during intimate moments is another question that is frequently asked. An open discussion with your partner usually resolves any concerns you may have. Some individuals simply choose to leave the pump in place. Others choose to use the longer tubing which allows them to place the pump well out of reach. Another idea is to temporarily disconnect from the pump and tubing. Just remember that disconnecting from the pump for long periods of time can result in high glucose levels that could lead to DKA. So, always be sure you reconnect the pump afterwards.

Talk to your healthcare professional about a plan including BG checks and possible correction boluses when disconnecting and reconnecting to your pump.




Should the pump be removed for X-rays, CT scans, and MRIs?



WARNING: Do not expose your pump to MRI equipment, diathermy devices, or other devices that generate strong magnetic fields (for example, x-ray, CT scan, or other types of radiation). The strong magnetic fields can cause the devices to malfunction and result in serious injury. If your pump is exposed to a strong magnetic field, discontinue use and contact your local representative for further assistance. Magnetic fields, and direct contact with magnets, may affect the accurate functioning of your system, which may lead to health risks such as hypoglycaemia or hyperglycaemia.

Cannula infusion sets such as the Quick-Set, Silhouette, and Mio can be left in place during the procedure. However, infusion sets that use a needle instead of a cannula to infuse insulin such as the Sure-T, must be removed prior to the procedure.

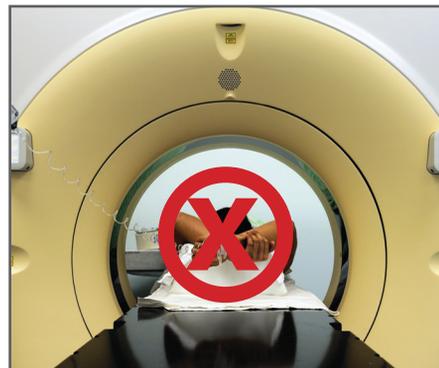

What do I need to know about traveling with my insulin pump?

Going through Airport Security

You can wear your insulin pump while going through an airport metal detector. If you are asked to go through a full body scanner, you must remove your insulin pump. **To avoid removing your devices, you may request an alternative screening process.**



WARNING: Do not send your devices through the x-ray machine as the radiation can make your pump nonfunctional or damage the part of the pump that regulates insulin delivery, possibly resulting in over delivery and hypoglycaemia.



Getting started | Frequently asked questions

Print and complete the information on your Medical emergency card to carry with you.

Notify security screeners that you have diabetes, that you are wearing an insulin pump and are carrying supplies with you. If there is any question, ask that they visually inspect the pump rather than removing it from your body. Remember, you may ask for a private screening if removal or lifting of clothing is required to display your pump.

General Travel Tips

- Pack extra supplies including reservoirs, infusion sets, batteries and ketone strips. Keep your supplies, insulin and a prescription with you, just in case your luggage is lost or your insulin becomes denatured. Consult with your airline for current regulations regarding flying with lithium batteries.



WARNING: Never store insulin in checked luggage as it may be exposed to extreme temperatures. Extreme heat or cold can cause insulin to lose its effectiveness which could result in hyperglycaemia.

- Pack glucose tablets or carbohydrate for treatment of low glucose. In case flights are delayed or canceled, pack extra food that is easy to carry, such as nutrition bars.
- While traveling outside of the country, you may want to take advantage of the Medtronic's travel loaner plan. This program allows you to take a "back-up" insulin pump with you when you travel. Contact your local representative to find out details about the travel loaner plan.





Getting started | Frequently asked questions

Always Be Prepared

When flying in an airplane, it is important that you stay connected to your pump and check your blood glucose more frequently. The routine hassle of travel, including stress, changes in time zones, schedules and activity levels, meal times and types of food, can all affect your diabetes control. Be extra attentive to your BG readings, and be prepared to respond if needed.



When traveling, make sure that you have backup syringes, vials of insulin or insulin pens (rapid-acting and long-acting insulin), and instructions from your healthcare provider should you need to return to insulin injections if your pump stops working.

Because travel rules are subject to change, passengers should consult their individual air carriers for regulations.



Getting started | Frequently asked questions

When should I call my healthcare professional?

Consult your healthcare professional about when, how often, and under what circumstances you should contact them. Typically, they will review your glucose information more frequently when you first start on pump therapy. This allows them to adjust and fine-tune your pump settings. Once adjusted, most healthcare professionals ask that you maintain a routine follow-up schedule. Examples of other situations that you should notify your healthcare professional about are:

Hypoglycaemia (BG less than 3.9 mmol/L)

- Any severe hypoglycaemic event that requires another person's assistance to treat the low; or any event that results in loss of consciousness.
- Frequent hypoglycaemia
- Hypoglycaemia that occurs around the same time each day or that routinely occurs after certain activities (such as vacuuming or washing the car)
- Hypoglycaemia that occurs after or during exercise



Hyperglycaemia (BG above your maximum target range or above 13.9 mmol/L)

- Hyperglycaemia that is frequent or persistent
- Hyperglycaemia that is accompanied by nausea or vomiting
- Hyperglycaemia and positive ketones
- Hyperglycaemia that occurs around the same time each day or routinely after a certain event (such as eating).

As always, when low or high blood sugars occur, follow the guidelines provided in the Safety Rules Quick Reference Guide in the Training Handouts section of this guide.





Notes

Use this space to write down any additional questions you might like to ask your healthcare professional.




Section 12: Additional features for experienced users

You have learned the features that are necessary to use your pump. There are additional features that you might find helpful. This section will discuss some additional menu options and features that are available on your insulin pump. Refer to the MiniMed 670G System User Guide for information about additional features and complete instructions for use.

Dual Wave and Square Wave bolus


The practice boluses that were given earlier were delivered as **Normal** boluses; that is, as a single immediate dose of insulin. This is the type of bolus you would typically use to cover normal food intake and to correct a high BG.

This pump also lets you deliver bolus insulin as a Dual Wave or Square Wave bolus. These can help better match the effects food has on your glucose levels.

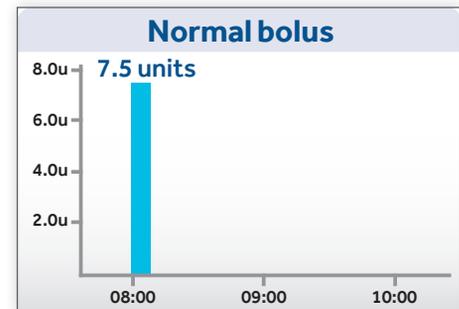

Turning Dual and Square Wave bolus on


- 1) Press .
- 2) Select **Options**.
- 3) Select **Delivery Settings**.
- 4) Select **Dual/Square Wave**.
- 5) Select **Dual Wave** to turn **On** if desired.
- 6) Select **Square Wave** to turn **On** if desired.
- 7) Select **Save**.

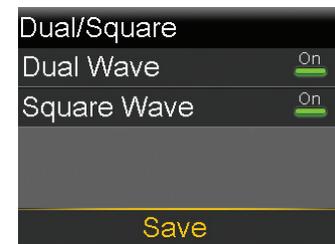

Square Wave

A Square Wave bolus delivers a bolus for an extended period of time. This can be helpful:

- to match delayed food digestion due to gastroparesis.
- for meals very low in carbohydrates but high in fat.
- when snacking on small amounts of carbs over a period of time, for example, at a reception.

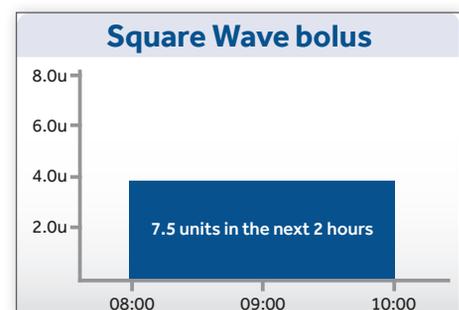

Getting started | Dual Wave and Square Wave bolus

When setting a Square Wave bolus, you will need to determine the duration that you want the bolus to deliver (30 minutes to 8 hours in 15 minute increments). This will vary depending on you individually, as well as the situation for which the Square Wave bolus is being used. Frequent glucose testing should be done until you and your healthcare professional have determined the best use for you.

Correction boluses calculated by the Bolus Wizard feature cannot be delivered as a Square Wave bolus since that insulin is needed right away.

Using Square Wave bolus...

Natalie eats at her desk at work and it takes her a while to finish because she often gets distracted. She delivers her lunch bolus as a Square Wave over 45 minutes to help make sure her insulin does not start to work before her carbs are digested.



▶ Giving a Square Wave bolus

This example will show a Square Wave bolus using the Bolus Wizard with a BG value of 5.6 mmol/L and 41 grams of carbs.

- 1) Press .
- 2) Select **Bolus**.
- 3) Select **Bolus Wizard**.
- 4) Enter BG and Carbs.
- 5) Select **Next**.
- 6) Press  and  to **Square** and press .

| | | |
|---------------------|------------|-------|
| Bolus Wizard | 09:00 | |
| BG | 5.6 mmol/L | 0.0 U |
| Active Ins. adjust. | | 0.0 U |
| Carbs | 41 g | 2.7 U |
| Bolus | | 2.7 U |
| Next | | |

| | |
|---------------|--------|
| Bolus Wizard | 09:00 |
| Bolus | 2.7 U |
| Dual | Square |
| Deliver Bolus | |

Getting started | Dual Wave and Square Wave bolus

- 7) Select Duration.
- 8) Press  to desired time and press .
- 9) Select Deliver Bolus.



Note: A **Square Bolus** banner will appear on the Home screen until bolus delivery is complete.



From the menu, select Bolus and you will see the following options:

- review bolus status, then press  to return to the menu.
- select Stop Bolus to stop delivery.
- select Bolus Menu to deliver a normal bolus while the square is delivering.




Dual Wave

A Dual Wave bolus combines the Normal and the Square Wave bolus. It delivers part of the bolus as a Normal Bolus (now) and part as a Square Wave bolus (over time).

A Dual Wave bolus can be helpful for meals high in both carbs and fat. Fat delays the digestion of carbs, meaning glucose does not enter the bloodstream right away. Giving some insulin as a normal bolus covers any immediate glucose rise. Giving the rest over time as a Square helps to match the delayed glucose rise.

When setting a Dual Wave bolus, you will need to determine:

- the percentage / amount of insulin you want delivered immediately and how much over time.
- the duration of time over which you want the Square portion delivered.

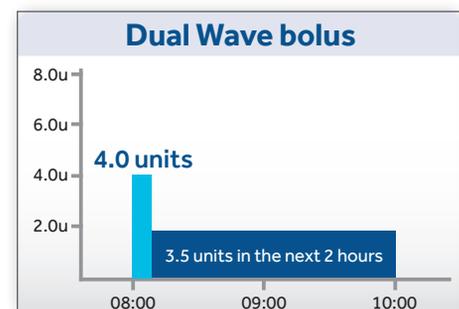

This will vary depending on you individually, as well as the types of food that are in the meal for which the Dual Wave bolus is being used. Frequent glucose testing should be done until you and your healthcare professional have determined the best use for you.

Getting started | Dual Wave and Square Wave bolus

▶ Giving a Dual Wave bolus

This example will show a Dual Wave bolus using the Bolus Wizard with a BG value of 7.3 mmol/L and 63 grams of carbs.

- 1) Press .
- 2) Select **Bolus**.
- 3) Select **Bolus Wizard**.
- 4) Enter BG and Carbs.
Notice in this example the total bolus for BG is 0.6 U and 4.2 U for carbs.
- 5) Select **Next**.
- 6) Press  to **Dual** and press .

| | | |
|---------------------|------------|-------|
| Bolus Wizard | | 09:00 |
| BG | 7.3 mmol/L | 0.6 U |
| Active Ins. adjust. | | 0.0 U |
| Carbs | 63 g | 4.2 U |
| Bolus | | 4.8 U |
| Next | | |

 **Note:** **Square** is not an option since a correction bolus was estimated so some insulin is needed now.

| | | |
|------------------|--|-------|
| Bolus Wizard | | 09:00 |
| Bolus | | 4.8 U |
| Dual Square | | |
| Deliver Bolus | | |

- 7) Select the Now/Square field and press  or  to change the amount of the bolus that is delivered **Now** and the amount delivered as **Square** if needed.
- 8) Select **Duration**.
- 9) Press  to desired time and press .
- 10) Select **Deliver Bolus**.

| | | |
|---------------|------|---------|
| Bolus Wizard | | 09:00 |
| Bolus | | 4.8 U |
| Now | 56 % | 2.7 U |
| Square | 44 % | 2.1 U |
| Duration | | 2:30 hr |
| Deliver Bolus | | |

 **Note:** Bolus for carbs is divided 50% Now/50% Square. Bolus for BG is added to Now.

 **Note:** A **Bolus (D)** banner that displays the bolus delivery progress will appear on the Home screen while the Now portion is delivering.

| | | |
|-----------|--|------------|
| BG | | 7.3 mmol/L |
| Bolus (D) | | 0.600 U |
| Total | | 4.800 U |

Getting started | Dual Wave and Square Wave bolus



Note: A **Dual Bolus** banner will appear on the Home screen until the Square delivery is complete.



From the menu select **Bolus** and you will see the following options:

- review bolus status, then press  to return to the menu.
- select **Stop Bolus** to stop delivery.
- select **Bolus Menu** to deliver a normal bolus while the square is delivering.



Using Dual Wave bolus...

When William ate pizza, his glucose level would be good for a while, but then 3 or 4 hours later it would be high. Now he uses a Dual Wave bolus to help reduce these post-meal highs.



Additional features | Temp Basal

Temp Basal

This feature lets you immediately increase or decrease your basal insulin for the period of time (duration) that you set. It is often used for exercise and sick days.

A Temp Basal can be set in either:

- **Percent:** delivers a percent of the current basal rate.
- **Rate:** delivers the amount that you enter.



A Temp Basal can be set to deliver more or less than your current basal rate. It can be set in any 30 minute increment for up to 24 hours.



Let's practice: Setting a Temp Basal

This example will show setting a Temp Basal to deliver 60% of the current basal rate for the next two hours.

- 1) Press
- 2) Select **Basal**.
- 3) Select **Temp Basal**.
- 4) Press to set duration and press .
- 5) Select **Next**.
- 6) Select **Percent**.
- 7) Press or to enter the percent of the current basal rate desired and then press .

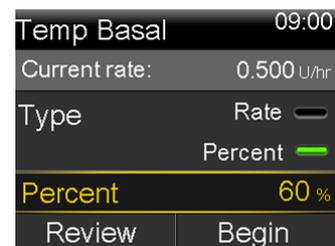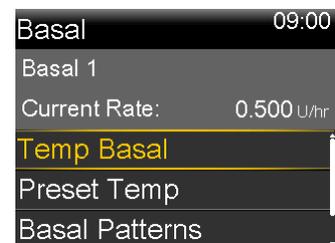

Note: If you choose to use Rate, press to Type and press . You can then enter the U/hr you want delivered.


- 8) Select **Begin**.

Additional features | Temp Basal

The Home screen displays a **Temp Basal** banner to indicate that you have a Temp Basal active.



From the menu select **Cancel Temp Basal** to review the details of the active Temp Basal.

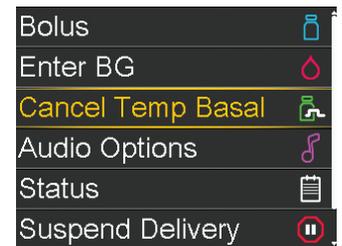

When the Temp Basal delivery is complete, the basal will automatically return to the regularly programmed basal rate.

Using a Temp Basal...


Patricia loves to work in her garden. She often finds, however, that her glucose levels run lower when she does. Now she uses a temp basal rate to decrease the amount of insulin she gets while she is working. This helps keep her glucose levels from dropping too low.



Let's practice: Cancelling a Temp Basal

If you need to return to your regularly programmed basal rate before your Temp Basal is completed, you can cancel it.

- 1) Press .
- 2) Select **Cancel Temp Basal**.

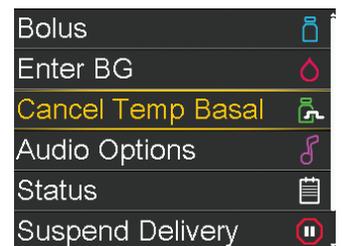

Additional features | Temp Basal

- 3) You can see the details about the Temp Basal. Select **Cancel Temp Basal**.

If you decide not to cancel, just press .

You can see that the Home screen no longer displays the Temp Basal banner.



Adding new or copying Basal Patterns

You may be using additional Basal Patterns. These are Basal Patterns set to account for days that require different basal amounts. For example, a pattern might be used for weekends because a person is less active than they are during the week. When setting an additional pattern, you can simply enter the basal rates into a new pattern, or you can copy and then make edits to a Basal Pattern that is already set. To enter another Basal Pattern, follow these steps:

- 1) Press .
- 2) Select **Basal**.
- 3) Press  and select **Delivery Settings**.
- 4) Press  and select **Basal Pattern Setup**.



Choose one of these two options:

How to add a new Basal Pattern

- 5) Press  and select **Add New**.
- 6) Select a name.
- 7) Enter times and basal rates for the additional pattern.
- 8) Select **Done**.
- 9) Press  to save.

How to Copy and Edit an existing Basal Pattern

- 5) Select **Basal 1** or another currently programmed Basal Pattern.
- 6) Select **Options**.
- 7) Press  to **Copy**. This copies the Basal Pattern that you have programmed and allows you to make the necessary changes.
- 8) Select name for this Basal Pattern.
- 9) Press  to **Edit**.
- 10) Continue by making the necessary changes to the programmed basal rates. To change active Basal Pattern, see *Changing which Basal Pattern is active on page 59*.
- 11) Select **Done** and press .
- 12) Press  to save.

Basal Patterns review

You will use the Basal Patterns option to do two things:

- Review the Basal Patterns that are currently set up.
- Choose the Basal Pattern that you wish to be active.



Let's practice: Reviewing Basal Patterns



- 1) Press
- 2) Select **Basal**.
- 3) Select **Basal Patterns**.
- 4) Select the Basal Pattern you wish to review.

- 5) Review basal rates.



Note: If you see a scroll bar on the right, press to see all basal rates in the Basal Pattern.

- 6) Select **OK**.

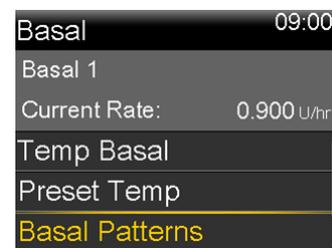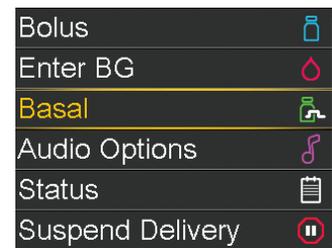



Let's practice: Changing which Basal Pattern is active

- 1) Press .
- 2) Select **Basal**.
- 3) Press  to **Basal Patterns** and press .
- 4) Select the Basal Pattern you want to make active.



Note: The checkmark indicates which Basal Pattern is active.

- 5) Select **Begin**.
- 6) Repeat step 1 through step 3 to see that the active Basal Pattern has changed.

| Basal Patterns | | 09:00 |
|----------------|---------|-------|
| Basal 1 | 19.25 U | ✓ |
| Day Off | 17.4 U | |

| Day Off | | 09:00 |
|---------------------|-------|-------------|
| 24 hr Total: 17.4 U | | |
| Start | End | Rate (U/hr) |
| 00:00 | 24:00 | 0.725 |
| Begin | | |



| Basal Patterns | | 09:00 |
|----------------|---------|-------|
| Basal 1 | 19.25 U | |
| Day Off | 17.4 U | ✓ |

Max Basal/Max Bolus

Max Basal

Max Basal is the maximum amount of basal insulin that can be delivered in one hour. Before you practice setting your Basal Patterns, you may need to change your Max Basal limit. Check your Max Basal setting on the pump you are currently using for your therapy. If your Max Basal is an amount other than 2.0 U/hr, follow these steps to change:

- 1) Press .
- 2) Select **Options** or **Basal**.
- 3) Select **Delivery Settings**.
- 4) Select **Max Basal/Bolus**.
- 5) Select **Max Basal**.
- 6) A screen will appear to ensure you are entering a value that has been determined by you and your healthcare professional. If this change has been recommended by your healthcare professional, press  and select **Continue**.
- 7) Select **Max Basal**.
- 8) Press  or  to enter number of U/hr and press .
- 9) Select **Save**.

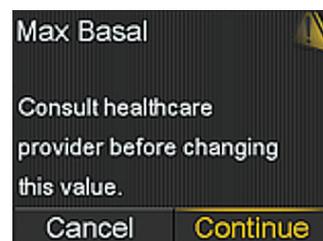
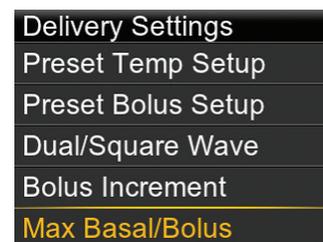


Note: Always consult your healthcare professional before adjusting your Max Basal setting..

Max Bolus

Before you continue, you may need to change your **Max Bolus** amount. Max Bolus is the maximum amount that can be given by any one bolus. Check your current pump settings. If your Max Bolus is an amount other than 10.0 U, follow these steps to change:

- 1) Press .
- 2) Select **Options** or **Bolus**.
- 3) Select **Delivery Settings**.
- 4) Select **Max Basal/Bolus**.
- 5) Select **Max Bolus**.
- 6) A screen will appear to ensure you are entering a value that has been determined by you and your healthcare professional. If this change has been recommended by your healthcare professional, press  and select **Continue**.
- 7) Select **Max Bolus**.
- 8) Press  or  to enter number of units and press .
- 9) Select **Save**.

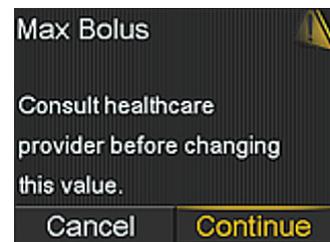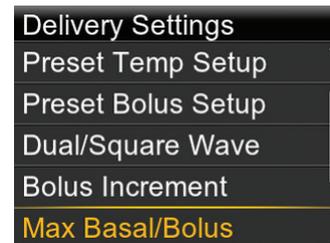

Note: Always consult your healthcare professional before adjusting your Max Bolus setting..

Auto Suspend

Auto Suspend is a safety feature that sounds an alarm and stops all insulin delivery if you do not press any buttons for the number of hours that you set. It is meant for situations where you are not responding to hypoglycaemia.

Auto Suspend is most useful if you live or travel alone. It is important to use if you have difficulty responding appropriately to lows, have hypoglycaemia unawareness, if you are susceptible to lows due to alcohol intake, or have a history or fear of lows at night.

Auto Suspend should be set based on your schedule. Let's say you typically go to bed about 23:00. At about 22:00 each evening you do a BG check and check your pump (buttons would be pressed). You usually get up at 07:00 and eat breakfast around 08:00. What happens if:

- Auto Suspend is set for 8 hours: Alarm would go off at 06:00 if no buttons had been pressed. Since you do not get up until 07:00, this could be a nuisance.
- Auto Suspend is set for 12 hours: Alarm would go off at 10:00 if no buttons had been pressed. You should have been up by now and given a bolus. If in a dangerous situation, receiving this alarm and stopping insulin could be very helpful.
- Auto Suspend is set for 18 hours: Alarm would go off at 16:00 if no buttons have been pressed. You should have been up and given bolus several hours ago. If in a dangerous situation, you may want to be alarmed and have delivery stopped sooner.

Choose the number of hours that seems right for you.



Setting Auto Suspend

- 1) Press .
- 2) Select **Options**.
- 3) Select **Delivery Settings**.
- 4) Select **Auto Suspend**.
- 5) Select **Alarm** to turn **On**.
- 6) Press  to **Time** and press .
- 7) Press  or  to change number of hours.
This example shows Auto Suspend set at 12 hours.
- 8) Press .
- 9) Select **Save**.



Using Auto Suspend...

Thomas is a runner and finds the days he runs, he is more prone to hypoglycaemia at night. He often sets a Temp Basal, but using Auto Suspend, he sleeps even more confidently because he knows his pump will stop delivering insulin and alarm if he is not waking up when he should.



Training handouts

Training handouts

This section contains handouts that you can use during or after your training.

- Safety Rules Quick Reference Guide
- Alerts
- Alarms
- Basal Quick Reference Guide
- Bolus Wizard™ Quick Reference Guide
- Changing the Quick-set™ infusion set
- Connecting the pump and meter

Feel free to remove these handouts and keep them in a place where they are easily accessible.

Safety Rules Quick Reference Guide

Glucose monitoring

Schedule for adjusting pump settings

When first starting pump therapy or any time pump settings need adjusting:

- Check your blood glucose (BG):
 - When you wake up
 - Before each meal
 - 2 hours after each meal
 - Bedtime
 - Mid-sleep or every 3–4 hours during sleep
- Do not eat between meals.



Checking BGs at these times provides the information needed to adjust and fine-tune pump settings as directed by your healthcare professional.

Schedule for routine monitoring

Once your pump settings are adjusted correctly and your glucose levels are stable, establish a routine that includes always checking your BG:

- When you wake up
- Before each meal
- Bedtime
- Occasionally mid-sleep
- Test more frequently during travel, times of stress, and illness



Treating low blood glucose levels

How to treat mild/moderate lows

15–15 Rule

If BG drops below 3.9 mmol/L:

1. Eat 15 grams of fast-acting carbohydrate.
2. Re-check BG in 15 minutes.
3. If BG is still below 3.9 mmol/L, repeat Steps 1 & 2 every 15 minutes until BG is within range.

Items that contain 15 grams:

- 3 to 4 glucose tablets
- 5 jelly beans
- 4 oz juice or soda (not diet)
- 8 oz milk (low or non-fat)
- 1 Tbsp sugar or honey

If BG is lower than 2.8 mmol/L, start treatment by eating 20 to 30 grams of carbohydrate or as otherwise directed by your healthcare professional.

How to treat a severe low

Keep a Glucagon Emergency Kit on hand in case a severe low occurs. Glucagon can be given by injection to raise glucose levels if you are unable to eat or drink to treat a low, or if you are unconscious.



A family member, co-worker, or friend should be instructed on how to give glucagon.



Note: If you are using continuous glucose monitoring (CGM), do not rely on sensor glucose values for making treatment decisions or the Suspend on low feature to prevent or treat a low blood glucose.

Safety Rules Quick Reference Guide

Treating high glucose levels

General guidelines: if BG is high but is lower than 13.9 mmol/L

1. Enter the BG reading into your pump.
2. Allow the Bolus Wizard™ feature to calculate the correction bolus amount.
3. Confirm the bolus amount and select **Deliver Bolus**.
4. Recheck your BG in one hour and again each hour until your BG is back within target range.

Never ignore high BG readings. Always consult the Bolus Wizard™ feature to see if a correction bolus should be taken.

General guidelines: if BG is higher than 13.9 mmol/L, check for ketones

If ketone test is negative:

1. Enter BG into pump or consult Bolus Wizard™ feature to see if correction dose is needed.
 - Use pump to give correction dose
2. Recheck BG in 1 hour
 - If BG is starting to decrease, continue to monitor until normal.
 - If BG is same or higher:
 - Give correction dose using a syringe.
 - Change infusion site, infusion set, reservoir, and insulin.
 - Continue to check BG every hour until BG returns to normal.

If ketone test is positive:

1. Take correction dose using a syringe.
2. Change infusion site, infusion set, reservoir, and insulin.
3. Troubleshoot pump.
4. Check BG every 1 to 2 hours. Give correction boluses as needed.
5. Drink non-carbohydrate fluids.
6. If BG continues to rise or if you have moderate to high ketones, nausea, vomiting, or difficulty breathing, notify physician or go to the nearest emergency room.

Diabetic ketoacidosis (DKA) prevention

Sick day guidelines

Illness or infection usually causes BGs to run higher than normal. Therefore, the risk of developing DKA is increased when you are ill.

Because DKA symptoms are similar to flu and stomach virus symptoms, check your BG and monitor for ketones often during illness.

- Check BG every 2 hours or as directed by your healthcare professional.
- Check urine or blood for ketones as directed by your healthcare professional.
- Immediately check ketones if you have nausea, vomiting, or abdominal pain.

- Notify doctor if ketones are positive, if you are unable to keep food down, or if no improvement within a few hours. Give a correction dose of insulin with a syringe according to your healthcare professional's recommendations and change infusion set and reservoir.

Check for ketones

Follow the instructions in your ketone testing kit.




Unexplained highs that do not decrease with a correction bolus may be caused by a dislodged or kinked infusion set or a weak vial of insulin.

Bolus Wizard™ is a trademark of Medtronic MiniMed, Inc. The glucagon design is a trademark of Eli Lilly and Company. © 2018 Medtronic MiniMed, Inc. All rights reserved.

Alerts

An alert makes you aware of a situation that may need your attention. When an alert occurs, you should check to see what your pump is telling you.

| Alert | When alert occurs | Steps to take |
|--|--|---|
| <p>Examples of alerts include Low reservoir, Low battery</p> | <p>Notification Light: The red light on the pump will blink once followed by a pause, blink again followed by a pause. This sequence continues until the alert is cleared. The flashing pattern is shown here:</p> <p style="text-align: center;">● ● ● ● ●</p> <p>Audio: Depending on your Audio Option settings, the pump emits a repeated alert tone, a continuous two-pulse vibration, or both.</p> <p>Display: The pump will display a notification with a yellow icon and instructions on what to do.</p> | <p>To address and clear the alert:</p> <ol style="list-style-type: none"> 1) Read the text on the screen to understand the alert and the steps that should be taken. 2) Press . 3) Press  on the desired option. |





The audio or vibration pattern repeats every 5 minutes or every 15 minutes (depending on the alert) until the alert is cleared.

Alarms

Alarms

When an alarm occurs, something has been detected that is preventing insulin from being delivered. You are not getting insulin. **It is important that you address an alarm right away.**

| Alarm | When alarm occurs | Steps to take |
|---|---|---|
| Examples of alarms include Insulin flow blocked and Replace battery now . | <p>Notification Light: The red light on the pump will blink twice, followed by a pause, blink twice again followed by a pause. This sequence continues until the alert is cleared. The flashing pattern is shown here:</p> <p>● ● ● ● ● ● ● ● ● ●</p> <p>Audio: Depending on your Audio Option settings, the pump emits a repeated alert tone, a continuous three-pulse vibration, or both.</p> <p>Display: The pump will display a notification with a red icon and instructions on what to do.</p> | <p>To address and clear the alarm:</p> <ol style="list-style-type: none"> 1) Read the text on the screen to understand the alarm and the steps that should be taken. 2) Press . 3) Press  on the desired option. |



The audio or vibration pattern repeats every minute for 10 minutes if the alarm is not cleared. **After 10 minutes, the alarm begins to siren.**



Note: An Insulin flow blocked alarm occurs when insulin cannot be pushed through the tubing or cannula. If this alarm occurs, make sure your reservoir is not empty and check the tubing for kinks, knots or other obvious blockages.


- If you detect an issue and are able to resolve it, check BG and select **Resume Basal**. If an Insulin flow blocked alarm occurs again, follow the steps on the screen and select **Rewind** to change your reservoir and infusion set.
- If you are unable to detect an issue, follow the steps on the screen and select **Rewind** to change your reservoir and infusion set.

Basal Quick Reference Guide

Change a basal rate

1. From the Home screen, press .


2. Select **Basal**.



3. Select **Delivery Settings**.



4. Select **Basal Pattern Setup**.



5. Select the Basal Pattern you wish to edit.



6. Select **Options**.

7. Select **Edit**.

8. Press  on the time segment.

9. Press  on **End** time.

10. Press  or  to change **U/hr** and press .



11. Select **Done**.




12. Review rates and select **Save**.



Reviewing Basal Patterns

1. From the Home screen, press .

2. Select **Basal**.



3. Select **Basal Patterns**.



4. Select the Basal Pattern you wish to review.



5. Review basal rates.

Note: If you see a scroll bar on the right, press  to see all basal rates in the Basal Pattern.




6. Select **OK**.

Add a basal rate to a Basal Pattern

1. From the Home screen, press .


2. Select **Basal**.



3. Select **Delivery Settings**.



4. Select **Basal Pattern Setup**.



Note: The basal rates shown are for illustration purposes only—your basal settings will be different.

Basal Quick Reference Guide

5. Select the Basal Pattern you are adding a rate to.
6. Select **Options**.
7. Select **Edit**.
8. Press  on the time segment.
9. Enter the new **End** time (this is the same as the start time of the basal rate you are adding) and press .



10. Press  if U/hr is not changing (Press  or  to change value and press .



11. Press  on the new time segment.
12. Press  to enter the new **End** time and press .
13. Press  to enter the new **Basal Rate** and press .
14. Continue adding end times and basal rates if necessary.



15. Select **Done**.
16. Review basal rates.
17. Select **Save**.




Temporary (Temp) basal rate


This feature lets you immediately increase or decrease your basal insulin for the period of time (duration) that you set. It is often used for exercise and sick days. A Temp Basal can be set in either Percent (delivers a percent of the current basal rate) or by Rate (delivers the amount that you enter).

Setting a Temp Basal

1. From the Home screen, press .
2. Select **Basal**.
3. Select **Temp Basal**.
4. Press  to set duration and press .
5. Select **Next**.
6. Select **Percent**.
7. Press  or  to enter the percent of current basal rate desired and press .



8. Select **Temp Basal**.
9. Press  to set duration and press .
10. Select **Next**.
11. Select **Percent**.
12. Press  or  to enter the percent of current basal rate desired and press .




Note: If you choose to use Rate, press  to Type and press .

13. Select **Begin**.



The Home screen displays a **Temp Basal** banner to indicate that you have a Temp Basal active.

From the menu select **Cancel Temp Basal** to review the details of the active Temp Basal.



When the Temp Basal is complete, the basal will automatically return to the regularly programmed basal rate.

Note: The basal rates shown are for illustration purposes only—your basal settings will be different.


Basal Quick Reference Guide

Cancel Temp Basal rate

If you need to return to your regularly programmed basal rate before your Temp Basal is completed, you can cancel it.

1. From the Home screen, press .

2. Select **Cancel Temp Basal**.



3. You can see the details about the Temp Basal.



Select **Cancel Temp Basal**.

If you decide not to cancel, just press .

You can see that the Home screen no longer displays the Temp Basal Banner.


Multiple Basal Patterns

Setting multiple Basal Patterns helps you more easily accommodate routine schedule changes that cause different basal needs (for example, weekday vs. weekend; day vs. night shift).

Set an additional Basal Pattern

1. From the Home screen, press .

2. Select **Basal**.



3. Select **Delivery Settings**.




4. Select **Basal Pattern Setup**.



5. Select **Add New**.

6. Select the name you would like to use.



7. Enter the basal rates needed for this pattern.



8. Select **Save**.


Note: The Basal pattern that your pump is currently using has a checkmark next to it.




How to change which Basal Pattern is Active

1. From Home screen, press .


2. Select **Basal**.



3. Select **Basal Patterns**.



4. Select the Basal Pattern you wish to be active.



Note: The checkmark indicates which Basal pattern is active.

5. Select **Begin**.




Note: The basal rates shown are for illustration purposes only—your basal settings will be different.

Bolus Wizard™ Quick Reference Guide


Entering your Bolus Wizard™ settings

Using either your most recent CareLink™ Personal settings report or your completed Setting Guide with your settings, follow these steps to enter your Bolus Wizard™ settings into your new pump.


- From the Home screen, press .
- Select **Options**.
- Select **Delivery Settings**.
- Select **Bolus Estimate Setup**.
- Select **Bolus Wizard** to turn on.



- Press  to continue reading text.
- Select **Next**.



- Review the description of Carb Ratio and select **Next**.



- Press  on the time segment.
- If you have only one Carb Ratio, press .



If you have more than one Carb Ratio, press  or  to enter the time that your Carb Ratio ends and the second begins and press .


- Press  or  to enter the **g/U** of your Carb Ratio and press .



If you have more than one Carb Ratio, continue by entering your time segments and Carb Ratios until all are entered.

- Select **Next**.

- Review the description of Sensitivity Factor and select **Next**.



- Press  on the time segment.



- If you have only one Sensitivity Factor, press .

If you have more than one Sensitivity Factor, press  or  to enter the time that your Sensitivity Factor ends and the second begins and press .


- Press  or  to enter the **mmol/L per U** of your Sensitivity Factor and press .



If you have more than one Sensitivity Factor, continue by entering your time segments and Sensitivity Factors until all are entered.

- Select **Next**.

- Review the description of BG Target and select **Next**.



- Press  on the time segment.



- If you have only one BG Target Range, press .

If you have more than one BG Target Range, press  or  to enter the time that your BG Target Range ends and the second begins and press .

Note: The boluses shown are for illustration purposes only—your settings and bolus results will be different.

Bolus Wizard™ Quick Reference Guide


- Press or to enter the Lo target and press .
- Press or to enter the Hi target and press .

If you have more than one BG Target Range, continue by entering your time segments and Lo and Hi targets until all are entered.

- Select **Next**.




- Review the description of Active Insulin Time and select **Next**.




- Select **Duration**.

- Press or to enter the **Duration** of your Active Insulin Time and press .



- Select **Save**.

The Bolus Wizard setup is now complete.



Deliver food and correction bolus

- Test BG.
 - Press .
- Select **Bolus > Bolus Wizard**.



- If using linked meter, **BG** is on screen. If not, select **BG**.
Press or to enter BG and press .



- Select **Carbs**.
- Press to enter grams of carbs and press .

- Select **Next**.



- Select **Deliver Bolus**.

Note: Active Ins. adjust. is the active insulin from previous boluses that is adjusted (subtracted) from the correction dose. In this example, there was no active insulin to subtract.



Deliver correction bolus—no food

- Test BG.
 - Press .
- Select **Bolus > Bolus Wizard**.



- If using linked meter, **BG** is on screen. If not, select **BG**.
Press or to enter BG and press .



- Press to **Next**.

- Select **Deliver Bolus**.



Note: In this example, there was active insulin to adjust—it was subtracted from the correction dose.

Deliver food bolus—no correction

- Press .
- Select **Bolus > Bolus Wizard**.



Note: The boluses shown are for illustration purposes only—your settings and bolus results will be different.

Bolus Wizard™ Quick Reference Guide

- Press to **Carbs** and press .
- Press to enter the amount of carbs you are eating and press .
- Select **Next**.
- Select **Deliver Bolus**.



Note: Active Insulin is never adjusted (subtracted) from a food bolus.

Checking bolus history



- Press .
Select **Options > History**.
- Select **Daily History**.
- Press on the day you would like to review.



Note: You can press the and arrows to move from day to day. You can also see further details by pressing on any item listed.


Edit Bolus Wizard™ settings

- Press .
Select **Options > Delivery Settings > Bolus Estimate Setup**.
- Select the setting to be changed.
- Select **Edit**.
- Press on the time segment. Press or to change the times or values.
- Select **Save**.



Review Bolus Wizard™ settings


- Press .
Select **Status > Settings Review**.
- Press to scroll through the list of settings.



Note: The boluses shown are for illustration purposes only—your settings and bolus results will be different.

MINIMED™ 670G SYSTEM | CHANGING THE QUICK-SET INFUSION SET QUICK REFERENCE GUIDE

START HERE



1  **2**  **3**  **4**   

Wash your hands.
Press **O**. Select **Options**.

Select **Reservoir & Tubing**.

Select **New Reservoir**.

Remove the infusion set you have been using by loosening the adhesive and pulling away from body.



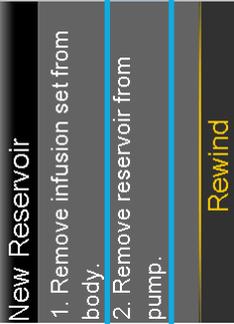

5   **6**   **New Reservoir**
1. Fill reservoir.
2. Connect tubing to reservoir.
DO NOT CONNECT TO BODY. **Next**

Remove the used reservoir from the pump.

Select **Rewind**.

FILL RESERVOIR & CONNECT TO THE INFUSION SET TUBING

Follow the next steps to fill reservoir with insulin and connect to the infusion set tubing.

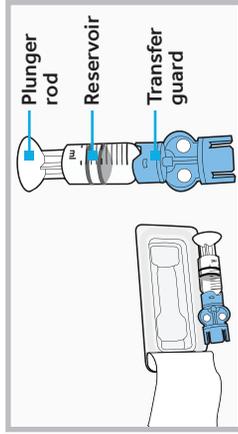1  **2**  **3**  **4** 


Remove from package. Make sure insulin vial is at room temperature to reduce the risk of air bubbles.

Pull plunger down to the amount that you plan to fill with insulin.


Wipe vial with alcohol. Place vial on table. Firmly press the blue transfer guard onto vial.

Push and hold plunger down.


WARNING If insulin or any liquid gets inside the tubing connector, it can temporarily block the vents that allow the pump to properly fill the infusion set. This may result in the delivery of too little or too much insulin, which could cause hyperglycemia or hypoglycemia.

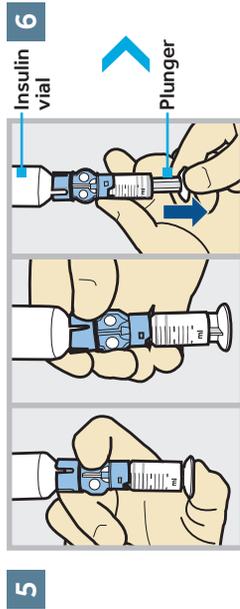


With your thumb still on the plunger, flip over so vial is on top. Release thumb and pull plunger down to fill with insulin.



Tap the reservoir to move air bubbles to top of reservoir. Push plunger up to move air into vial.




If needed, pull plunger back down to amount of insulin needed for 2-3 days.




To avoid getting insulin on the top of the reservoir, turn vial over so it is upright. Hold transfer guard and turn reservoir counter-clockwise and remove from transfer guard.

CONNECT RESERVOIR TO INFUSION SET


You will place the tubing connector onto the end of the infusion set to the filled reservoir.

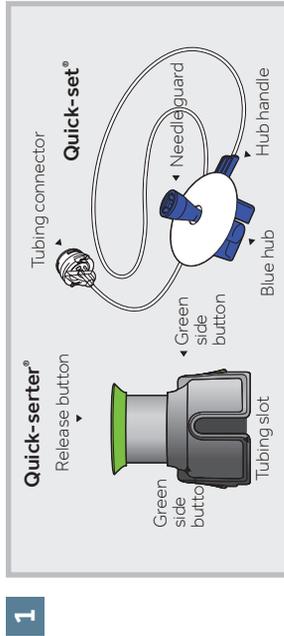


Remove infusion set from package. Remove the paper that holds the tubing together.

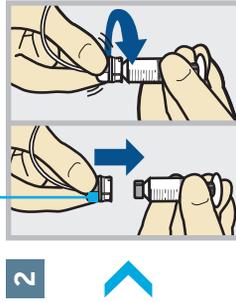

Gently push the tubing connector onto reservoir. Turn clockwise until locked. You will hear a click.



If you see air bubbles, tap reservoir to move them to top. Push plunger just a bit to move them into tubing.




Twist plunger counter-clockwise to loosen and remove.




THE BACKLIGHT MAY HAVE TURNED OFF
Press any button to turn the screen back on.

Press **O** to open the menu. If the pump is locked, you will need to unlock the pump after pressing **O**.

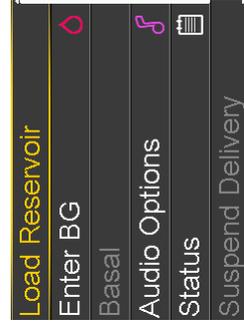

Select **Load Reservoir** from the menu.


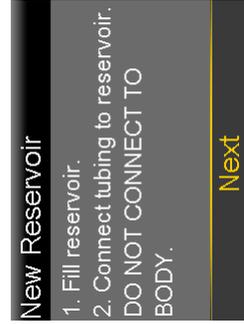


Select **Next**.
Continued on next page

PLACE RESERVOIR INTO PUMP

Now place the filled reservoir into the reservoir compartment of the pump.

1 **New Reservoir**
 3. Place reservoir into pump and lock.
DO NOT CONNECT TO BODY.
Next



Place reservoir into pump.

Turn clockwise until you feel reservoir lock into place.

3 **New Reservoir**
 3. Place reservoir into pump and lock.
DO NOT CONNECT TO BODY.
Next

Select **Next**.


LOAD RESERVOIR AND FILL TUBING

Follow these steps to load the reservoir and fill the tubing.

1 **Load Reservoir**
 Select Load and hold until complete.
DO NOT CONNECT TO BODY.
Load **Next**

2 **Load Reservoir**
 Complete
DO NOT CONNECT TO BODY.
Load **Next**

3 **Fill Tubing**
DO NOT CONNECT TO BODY.
 Hold Fill until drops appear. Then select **Next**.
0.0_U
Fill **Next**



4 **Fill Tubing**
DO NOT CONNECT TO BODY.
 Hold Fill until drops appear. Then select **Next**.
11.3_U
Fill **Next**

Select **Load** and keep holding **O**.

When you see this screen, select **Next**.



Select **Fill** and keep holding **O** until you see drops at the end of tubing, then let go.

After you see drops, press **>** and select **Next**.

INSERT INFUSION SET

Next, follow the steps to insert the infusion set into your body.


Fill Cannula?
 1. Insert infusion set into body.
 2. Select Fill to fill cannula or Done if not needed.
Fill **Done**

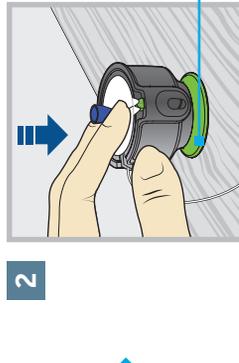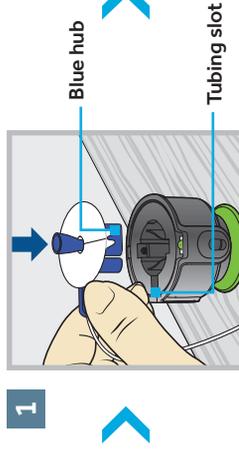

Place blue hub into serter, placing the handle in the tubing slot.


Holding the serter with one hand, gently press infusion set to secure. Be careful not to push all the way into serter. Do not hold or press on the release button.

Continued on next page

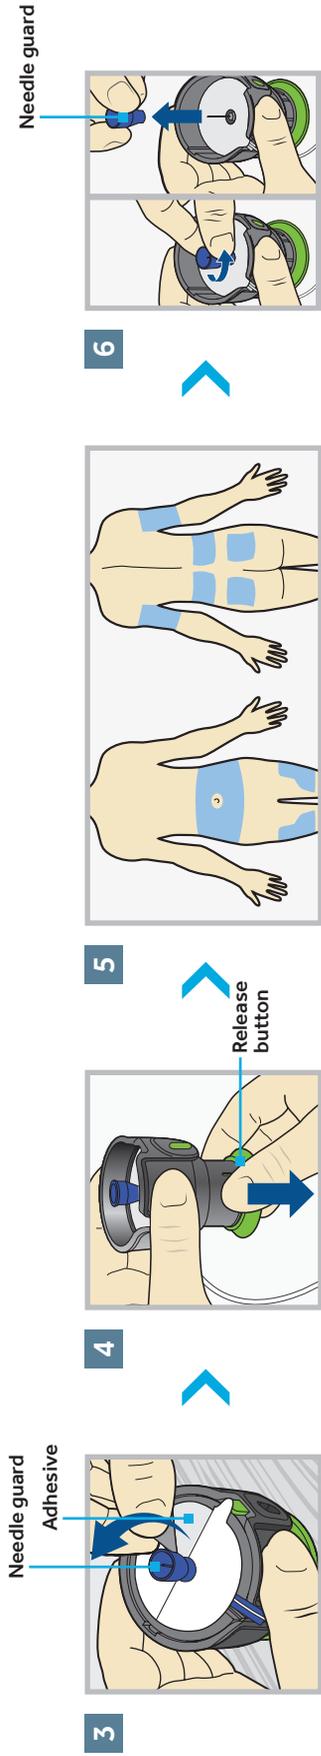


3

Holding needle guard, pull off the paper that covers the adhesive.



4

Pull green handle down until you hear it click.

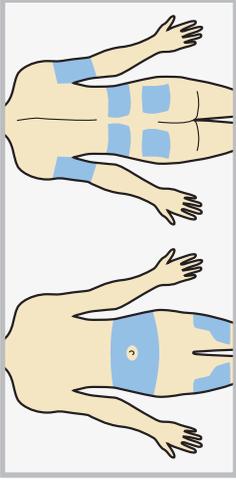


5

Choose an insertion site from the shaded areas shown here. Wipe with alcohol or other antiseptic.




6

Turn to loosen needle guard and pull.

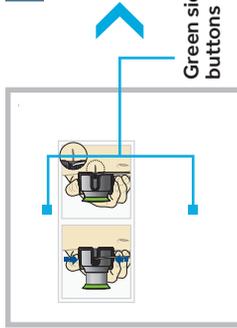


7

Hold serter against cleaned site.

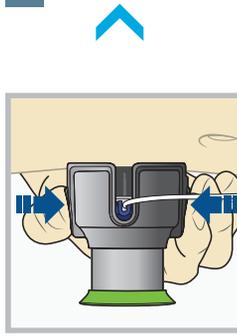


8

Press the two green side buttons at the same time.




9

Press down the release button to unlock.




10

Pull serter away from body. Press adhesive against skin.

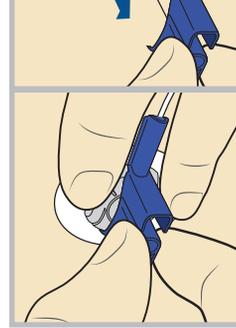

11

Hold infusion set. Pull blue handle straight out to remove needle.





12

Fold blue handle until locked.

FILL CANNULA

You will now fill the cannula, the little tube under your skin, with insulin.

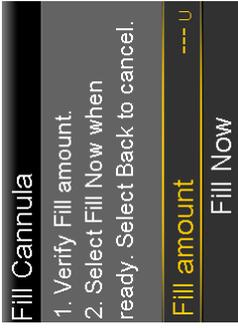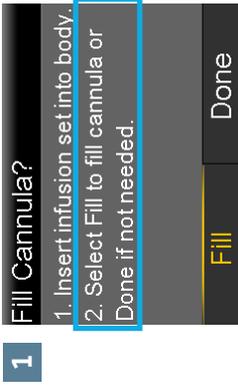

NOTE: Your pump will remember the **Fill amount** that you used last. Always verify that the Fill amount is correct.


- If it is correct, press **✓** to **Fill Now** and press **○**.
- If it is incorrect, press **○**. Change to correct amount and press **○**. Select **Fill now**.

Select **Fill**.

Select **Fill amount** and enter :

- 0.300 if using 6mm cannula
- 0.500 if using 9mm cannula

Then press **○**.

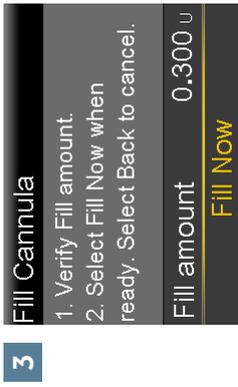

NOTE: Select **Stop Filling** if you need to stop, for example, if you notice the **Total** amount is incorrect. This should rarely happen if you have verified the **Fill amount** on the previous screen.

Select **Fill Now**.

The Home screen displays the insulin as it fills the cannula.

Your infusion set change is now complete!

Connecting the pump and meter


1. Hold the Menu button until the meter turns on.



2. Scroll to your language and press **OK**. Press **OK** to confirm.



3. Press **OK** when asked **Connect to a MiniMed™ Pump?**



4. Press **OK**.



5. Press **Auto Connect**.

Put the meter down and pick up your pump.



6. Press **⊙**.



7. Select **Options**.

8. Select **Utilities**.

9. Select **Device Options**.

10. Select **Connect Device**.





11. Select **Auto Connect** on your pump.

12. Press **✓**.

13. Press **➤**.

14. Select **Continue**.


Place the meter and pump next to each other.



15. Select **Search** on your pump.



16. Select **Search** on your meter. *The search may take up to 2 minutes.*



17. Check to see that the Device SN (serial number) on the pump screen matches the Device SN on the meter.



18. If they match select **Confirm** on the pump.




19. Check to see that the SN on the back of the pump matches the SN now on the meter screen.



20. Select **Next** on the meter.



21. Press **Always**.*




22. Then press **OK**.

23. Select the desired **Date Format**.



24. Press **OK**.
If time and date are not correct you must change them on the pump.



25. Press **Accept** to select **AutoLog is Off**.
*AutoLog allows you to mark a test result as Before Meal, After Meal or Fasting.**



26. **Accept** or **Change** High and Low Alerts.*



27. **Accept** or **Change** the Target Range.* Press **Accept** again to confirm.



28. Setup is now complete and you are ready to use the meter.



*For more detail on this feature see your meter guide.



Notes





Notes





**Medtronic Diabetes 24-hour toll free helpline
(Australian landlines): 1800 777 808**

www.medtronic-diabetes.com.au

**Medtronic Australasia Pty Ltd
2 Alma Road, Macquarie Park NSW 2113 Australia**

Please note: In contacting the Diabetes Toll Free, your personal and health information may be disclosed to an operator located outside Australia.

©2018 Medtronic Australasia Pty Ltd. All rights reserved. Medtronic, Medtronic logo and Further, Together are trademarks of Medtronic.™

***Third party brands are trademarks of their respective owners. All other brands are trademarks of a Medtronic company. Bolus Wizard™, CareLink™, Dual Wave™, MiniMed™, Mio™, Quick-set™, Silhouette™, Square Wave™, and Sure-T™ are trademarks of Medtronic.**

Ascensia, the Ascensia Diabetes Care logo, and CONTOUR are trademarks of Ascensia Diabetes Care. 5190-082018

Medtronic
Further, Together