
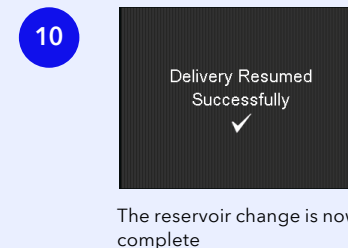
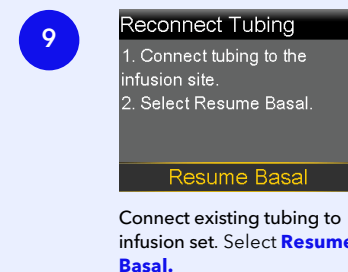


 **Avoid reservoir and infusion set changes before bed.**
Check glucose levels for 2 hours after changing infusion set.

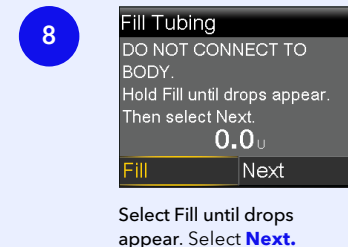

Medtronic Australasia Pty Ltd

Level 8, 11 Khartoum Street Macquarie Park,
 NSW 2113, Australia
 Tel: +61 2 9857 9000
 Fax: +61 2 9889 5167
 Toll Free: 1800 777 808

E-Mail: australia.diabetes@medtronic.com Facebook: www.facebook.com/MedtronicDiabetesAUS
 YouTube: Medtronic Diabetes ANZ
<https://www.medtronic-diabetes.com.au/>

Always read the instructions for use.

For detailed information regarding the instructions for use, indications, contraindications, warnings, precautions, and potential adverse events, please consult the device manual. For further information, contact your local Medtronic representative.